medRxiv preprint doi: https://doi.org/10.1101/2019.12.11.19014571; this version posted December 15, 2019. The copyright holder for this preprint (which was not certified by peer review) is the author/funder, who has granted medRxiv a license to display the preprint in perpetuity.
It is made available under a CC-BY-NC-ND 4.0 International license .

Review

Brain-Computer Interface Robotics for Hand Rehabilitation After Stroke: A Systematic Review

Paul Dominick E Baniqued[1*], Emily C Stanyer[2], Muhammad Awais[2], Ali Alazmani[1], Andrew E Jackson[1], Mark A Mon-Williams[2], Faisal Mushtaq[2], Raymond J Holt[1]

1 School of Mechanical Engineering, University of Leeds, LS2 9JT Leeds, United Kingdom

2 School of Psychology, University of Leeds, LS2 9JZ Leeds, United Kingdom

*Correspondence: mnpdeb@leeds.ac.uk

NOTE: This preprint reports new research that has not been certified by peer review and should not be used to guide clinical practice.

medRxiv preprint doi: https://doi.org/10.1101/2019.12.11.19014571; this version posted December 15, 2019. The copyright holder for this preprint (which was not certified by peer review) is the author/funder, who has granted medRxiv a license to display the preprint in perpetuity.
It is made available under a CC-BY-NC-ND 4.0 International license .

Abstract

Background: Electroencephalography-based brain-computer interfaces (BCI) that allow the control of robotic devices to support stroke patients during upper limb rehabilitation are increasingly popular. Hand rehabilitation is focused on improving dexterity and fine motor control and is a core approach for helping stroke survivors regain activities of daily living. This systematic review examines recent developments in BCI-robotic systems for hand rehabilitation and identifies evidence-based clinical studies on stroke patients.

Methods: A search for January 2010-October 2019 articles using Ovid MEDLINE, Embase, PEDro, PsycINFO, IEEE Xplore and Cochrane Library databases was performed. The selection criteria included BCI-hand robotic systems for rehabilitation in various development stages involving tests on healthy human subjects or stroke survivors. Data fields include those related to study design, participant characteristics, technical specifications of the system, and clinical outcome measures.

Results: 30 studies were identified as eligible for qualitative review and among these, 11 studies involved testing a BCI-hand robot on chronic and subacute stroke patients. Statistically significant improvements in motor assessment scores relative to controls were observed for two BCI-hand robot interventions. The degree of robot control for the majority of studies was limited to triggering the device to perform grasping or pinching movements using motor imagery. Most employed a combination of kinaesthetic and visual response via the robotic device and display screen, respectively, to match feedback to motor imagery.

Conclusion: Most studies on BCI-robotic systems for hand rehabilitation report systems at prototype or pre-clinical stages of development. Some studies report statistically significant improvements in functional recovery after stroke, but there is a need to develop a standard protocol for assessing technical and clinical outcomes so that the necessary evidence base on efficiency and efficacy can be developed.

medRxiv preprint doi: https://doi.org/10.1101/2019.12.11.19014571; this version posted December 15, 2019. The copyright holder for this preprint (which was not certified by peer review) is the author/funder, who has granted medRxiv a license to display the preprint in perpetuity.
It is made available under a CC-BY-NC-ND 4.0 International license .

Keywords: brain-computer interface, electroencephalography, motor imagery, action observation, robot-assisted rehabilitation, hand, wrist, stroke, therapy

Background

There is growing interest in the use of robotics within the field of rehabilitation. This interest is driven by the increasing number of people requiring rehabilitation following problems such as stroke (with an ageing population), and the global phenomenon of insufficient numbers of therapists able to deliver rehabilitation exercises to patients [1,2]. Robotic systems allow a therapist to prescribe exercises that can then be guided by the robot rather than the therapist. An important principle within the use of such systems is that the robots assist the patient to actively undertake a prescribed movement rather than the patient's limb being moved passively. This means that it is necessary for the system to sense when the patient is trying to generate the required movement (given that, by definition, the patient normally struggles with the action). One potential solution to this issue is to use force sensors that can detect when the patient is starting to generate the movement (at which point the robot's motors can provide assistive forces). It is also possible to use measures of muscle activation (EMGs) to detect the intent to move [3]. There is, however, growing interest in the potential of using measures of brain activity to identify when a patient is trying to generate a movement- referred to as Brain Computer Interfaces, or BCIs. This interest in BCIs is motivated by idea that the rehabilitation process can be enhanced by particular types of brain activity related to imagining the movement [4]. There is a long history of using robotic devices for stroke rehabilitation [5,6] and in the last decade, there has been a concerted effort by groups of clinicians, neuroscientists and engineers to integrate these systems with incoming brain signals to enhance the efficacy and effectiveness of stroke rehabilitation. The purpose of this

medRxiv preprint doi: https://doi.org/10.1101/2019.12.11.19014571; this version posted December 15, 2019. The copyright holder for this preprint (which was not certified by peer review) is the author/funder, who has granted medRxiv a license to display the preprint in perpetuity.
It is made available under a CC-BY-NC-ND 4.0 International license .

manuscript is to review the current state-of-the-art of existing brain-computer 'closed loop' interfaces in terms of the technological readiness of existing systems, and the evidence for their clinical effectiveness.

BCIs allow brain state-dependent control of robotic devices to aid stroke patients during upper limb therapy and have been gaining research attention since their first implementation more than a decade ago [7,8]. Graimann et al. [4] defined a BCI as an artificial system that provides direct communication between the brain and a device based on the user's intent; bypassing the normal efferent pathways of the body's peripheral nervous system. A BCI recognises user intent by measuring brain activity and translating it into executable commands usually performed by a computer, hence the term "brain-computer interface".

Most robotic devices used in upper limb rehabilitation exist in the form of exoskeletons or end-effectors. Robotic exoskeletons (i.e., powered orthoses, braces) are wearable devices where the actuators are biomechanically aligned with the wearer's joints and linkages; allowing the additional torque to provide assistance, augmentation and even resistance during training [9]. In comparison, end-effector systems generate movement through applying forces to the most distal segment of the extremity via handles and attachments [9]. Rehabilitation robots are classified as Class II-B medical devices (i.e., a therapeutic device that administers the exchange of energy, mechanically, to a patient) and safety considerations are important during development [10,11]. Most commercial robots are focused on arms and legs, each offering a unique therapy methodology. There is also a category of device that target the hand and finger. Hand and finger rehabilitation are core component in regaining activities of daily living (ADL) as many ADLs require dexterous and fine motor movements (e.g. grasping and

medRxiv preprint doi: https://doi.org/10.1101/2019.12.11.19014571; this version posted December 15, 2019. The copyright holder for this preprint (which was not certified by peer review) is the author/funder, who has granted medRxiv a license to display the preprint in perpetuity.
It is made available under a CC-BY-NC-ND 4.0 International license .

pinching). Thus, the current review is focused on devices that have been designed specifically for wrist, hand and finger rehabilitation.

The potential of BCIs has gained considerable attraction because the neural activity involved in the control of the robotic device may be a key component in the rehabilitation itself. For example, mental rehearsal of movement is thought to activate some of the neural networks involved in movement execution (ME) [12–15]. The resulting rationale is that encouraging the use of motor imagery (MI) (i.e., the imagination of movement without execution) could increase the capacity of the motor cortex to control major muscle movements and decrease the necessity to use neural circuits damaged post-stroke. The scientific justification for this approach was first provided by Jeannerod [15] who suggested that the neural substrates of MI are part of a shared network that is also activated during the simulation of action by the observation of action (AO) [15]. These 'mirror neuron' systems are thought to be an important component of motor control and learning [15] - hence the belief that stimulating these systems could aid rehabilitation.

A recent meta-analysis of the neural correlates of action (MI, AO and ME) quantified 'conjunct' and 'contrast' networks in the cortical and subcortical regions [12]. This analysis, which took advantage of open-source historical data from fMRI studies, reported consistent activation in the premotor, parietal and somatosensory areas for MI, AO and ME. Predicated on such data, researchers have reasoned that stimulating MI should cause activation of the neural substrates that are also involved in controlling movement and there have been a number of research projects that have used AO in combination with MI in neurorehabilitation [16–18] and motor learning studies [19,20] over the last decade.

medRxiv preprint doi: https://doi.org/10.1101/2019.12.11.19014571; this version posted December 15, 2019. The copyright holder for this preprint (which was not certified by peer review) is the author/funder, who has granted medRxiv a license to display the preprint in perpetuity.
It is made available under a CC-BY-NC-ND 4.0 International license .

The strategy of BCI-robot systems in rehabilitation is to recognise the patient's intention to move or perform a task via an electroencephalography acquisition system [21], and then use the robotic device to provide assistive forces in a manner that mimics the actions of a therapist during standard therapy sessions [22]. The resulting feedback is patient-driven and is designed to aid in closing the neural loop from intention to execution. This process is said to promote use-dependent neuroplasticity within intact brain regions and relies on the repeated experience of initiating and achieving a specified target [23,24]; making the active participation of the patient in performing the therapy exercises an integral part of the motor re-learning process [25,26]. It is important to note that whilst the rationale underpinning the conjecture that BCI-robot systems could be useful in hand rehabilitation is reasonable, it is just a conjecture that requires empirical support.

Electroencephalography (EEG) is currently the instrument of choice for data acquisition in BCI systems because it is non-invasive, easy to use and can detect relevant brain activity with high temporal resolution [27,28]. In principle, the recognition of MI activity via EEG can allow the control of a device independent of muscle activity [4]. It has been shown that MI-based BCI can discriminate motor intent by detecting event-related spectral perturbations (ERSP) [21,29] and/or event-related desynchronisation/synchronisation (ERD/ERS) patterns in the μ (9-11 Hz) and β (14-30 Hz) sensorimotor rhythm of EEG signals [29]. However, EEG also brings with it some challenges- these neural markers are often concealed by various artefacts and may be difficult to recognise through the raw EEG signal alone. Thus, signal processing (via feature extraction and classification) is a vital part of obtaining a good MI signal for robotic control.

medRxiv preprint doi: https://doi.org/10.1101/2019.12.11.19014571; this version posted December 15, 2019. The copyright holder for this preprint (which was not certified by peer review) is the author/funder, who has granted medRxiv a license to display the preprint in perpetuity.
It is made available under a CC-BY-NC-ND 4.0 International license .

One implication of using MI and AO to justify the use of BCI approaches is that great care must be taken with regard to the quality of the environment in which the rehabilitation takes place. An important feature of MI is that, by definition, the patient must be able to imagine the movement. Likewise, AO requires the patients to clearly see the action. This suggests that the richness and vividness of the visual cues provided is an essential part of an effective BCI system. It is also reasonable to assume that feedback is important within these processes and thus the quality of feedback should be considered as essential. Finally, motivation is known to play an important role in promoting active participation during therapy [26,30]. Thus, a good BCI system should incorporate an approach (such as gaming and positive reward) that increases motivation. Recent advances in technology make it far easier to create a rehabilitation environment that provides rich vivid cues, gives salient feedback and is motivating. For example, the rise of immersive technologies, including virtual reality (VR) and augmented reality (AR) platforms [31,30,32], allows for the creation of engaging visual experiences that have the potential to improve a patient's self-efficacy [33] and thereby encourage the patient to maintain the rehabilitation regime. One specific example of this is visually amplifying the movement made by a patient when the movement is of limited extent so that the patient can see their efforts are producing results [34].

In this article, we review the development of BCI-robotic systems for hand rehabilitation and capture clinical studies involving stroke patients. Our goal was to address three critical questions for understanding the current value and potential of BCI-based robotic therapy:

(1) Identify how BCI technologies are being utilised in controlling robotic devices for hand rehabilitation. Our focus was on the study design and the tasks that are employed in setting up a BCI-hand robot therapy protocol.

medRxiv preprint doi: https://doi.org/10.1101/2019.12.11.19014571; this version posted December 15, 2019. The copyright holder for this preprint (which was not certified by peer review) is the author/funder, who has granted medRxiv a license to display the preprint in perpetuity.
It is made available under a CC-BY-NC-ND 4.0 International license .

(2) Document the state-of-art of BCI systems. Because BCI for rehabilitation is still an emerging field of research, we expected that most studies would be in their proof-of-concept or clinical testing stages of development. Our purpose was to determine the limits of this technology in terms of: (a) resolution of hand MI detection and (b) the degree of which we can have robotic control.

(3) Evaluate the clinical significance of BCI-hand robot systems by looking at the outcome measures in motor recovery and determine if a standard protocol exists for these interventions.

It is important to note that there have been several recent reviews exploring BCI for stroke rehabilitation. For example, Monge-Pereira et al. [35] compiled EEG-based BCI studies for upper limb stroke rehabilitation. Their systematic review (involving 13 clinical studies on stroke and hemiplegic patients) reported on research methodological quality and improvements in the motor abilities of stroke patients. Cervera et al. [36] performed a meta-analysis on the clinical effectiveness of BCI-based stroke therapy among 9 randomised clinical trials (RCT). McConnell et al. [37] reviewed and provided insights from a total of 110 robotic devices with brain-machine interfaces for hand rehabilitation post-stroke. These reviews, in general, have reported that such systems provide improvements in both functional and clinical outcomes in pilot studies or trials involving small sample sizes. Thus, the literature indicates that EEG-based BCI are a promising general approach for rehabilitation post-stroke.

The current work complements these previous reports by focusing on a systematic review of the rehabilitation of the fine motor skills associated with hand movement, and profiling BCI-robot systems for the hands with their corresponding technical and clinical implementations.

medRxiv preprint doi: https://doi.org/10.1101/2019.12.11.19014571; this version posted December 15, 2019. The copyright holder for this preprint (which was not certified by peer review) is the author/funder, who has granted medRxiv a license to display the preprint in perpetuity.
It is made available under a CC-BY-NC-ND 4.0 International license .

Methods

Protocol Registration

Details of the protocol for this systematic review were registered on the International Prospective Register of Systematic Reviews (PROSPERO) and can be accessed at www.crd.york.ac.uk/PROSPERO (ID: CRD42018112107).

Search Strategy and Eligibility

An in-depth search of articles from January 2010 to October 2019 was performed on Ovid MEDLINE, Embase, PEDro, PsycINFO, IEEE Xplore and Cochrane Library. Only full-text articles published in English were selected for this review. Table 1 shows the combination of keywords used in the literature searching.

Table 1. Keyword Combinations

Set 1 (OR)		Set 2 (OR)		Set 3 (OR)
Brain-computer interface/BCI Electroencephalography/EEG Brain-machine interface/BMI Neural control interface Mind-machine interface	AND	Stroke (rehabilitation/ therapy/treatment/recovery) Motor (rehabilitation, therapy/treatment/recovery) Neurorehabilitation Neurotherapy Hand (rehabilitation/therapy/ recovery/exercises/movement)	AND	Robotic (exoskeleton/ orthosis) Powered (exoskeleton/ orthosis) Robot Device

The inclusion criteria for the articles were: (1) publications that reported the development of an EEG-based BCI; (2) studies targeted towards the rehabilitation of the hand after stroke; (3) studies that involved the use of BCI and a robotic device (e.g., exoskeleton, end-effector type, platform-types, etc.); (4) studies that performed a pilot test on healthy human subjects or a clinical trial with stroke patients. The articles were also screened for the following exclusion

medRxiv preprint doi: https://doi.org/10.1101/2019.12.11.19014571; this version posted December 15, 2019. The copyright holder for this preprint (which was not certified by peer review) is the author/funder, who has granted medRxiv a license to display the preprint in perpetuity.
It is made available under a CC-BY-NC-ND 4.0 International license .

criteria: (1) studies that targeted neurological diseases other than stroke; (2) studies that used other intention sensing mechanisms (electromyography/EMG, electrooculography/EOG, non-paretic hand, other body parts, etc.).

Two authors performed independent screenings of titles and abstracts based on the inclusion and exclusion criteria. The use of a third reviewer was planned a priori in cases where a lack of consensus existed around eligibility. However, consensus was achieved from the first two authors during this stage. Full-text articles were then obtained, and a second screening was performed until a final list of studies was agreed to be included for data extraction.

Data Extraction

The general characteristics of the study and their corresponding results were extracted from the full-text articles by the reviewers following the Preferred Reporting Items for Systematic Reviews and Meta-Analysis (PRISMA) checklist. Data fields included those related to study design, participant characteristics, technical specifications of the system, and technical and experimental results. For studies involving stroke patients, clinical outcomes were obtained based on muscle improvement measures such as Fugl-Meyer Motor Assessment (FMMA) scores [38], Action Research Arm Test (ARAT) scores [39], United Kingdom Medical Research Council (UK-MRC) muscle grade [40], Grip Strength (GS) Test and Pinch Strength (PS) Test scores (i.e., kilogram force collected using an electronic hand dynamometer) among others.

medRxiv preprint doi: https://doi.org/10.1101/2019.12.11.19014571; this version posted December 15, 2019. The copyright holder for this preprint (which was not certified by peer review) is the author/funder, who has granted medRxiv a license to display the preprint in perpetuity.
It is made available under a CC-BY-NC-ND 4.0 International license .

Quality Assessment

Technological Readiness

We first assessed the development stages of the systems used in the studies extracted. By performing a Technological Readiness Assessment (TRA), we were able to determine the maturity of the systems via a Technology Readiness Level (TRL) scale of 1-9 and quantify its implementation in a research or clinical setting. Since a BCI-robot for rehabilitation can be categorised as a Class II-B medical device we have adapted a customised TRL scale to account for these requirements [41].

Clinical Use

A methodological quality assessment was also performed for clinical studies based on the Physiotherapy Evidence Database (PEDro) Scale [42]. This scale evaluates studies with a checklist of 11 items based on experts' consensus criteria in physiotherapy practice. The complete details of the criteria can be found online [43]. A higher score in the PEDro scale (6 and above) implied better methodological quality but are not used as a measure of validity in terms of clinical outcomes. Pre-defined scores from this scale were already present in studies appearing in the PEDro search. However, studies without PEDro scores or are not present in the PEDro database at all had to be manually evaluated by the authors against the 11-item checklist (five of seven studies).

medRxiv preprint doi: https://doi.org/10.1101/2019.12.11.19014571; this version posted December 15, 2019. The copyright holder for this preprint (which was not certified by peer review) is the author/funder, who has granted medRxiv a license to display the preprint in perpetuity.
It is made available under a CC-BY-NC-ND 4.0 International license .

Results

Search Results

Figure 1 shows the study selection process and the number of articles obtained at each stage.

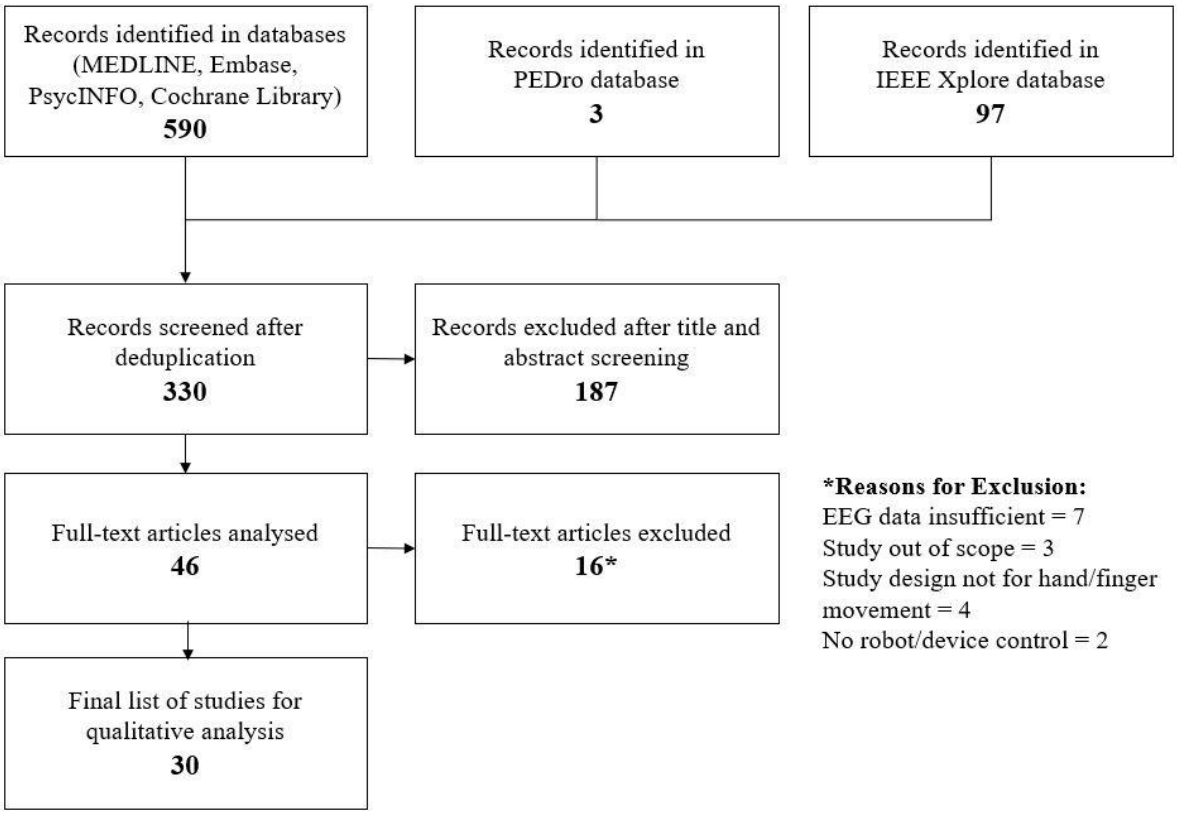

Figure 1. Study Selection Flowchart

A total of 590 studies were initially identified. After deduplication, 330 studies underwent title and abstract screening. Forty six studies passed this stage and among these, 16 were removed after full-text screening due to the following reasons: insufficient EEG and robotic data [44–50], the study was out of scope [51–53], the study design was not for hand/finger movement [54–57], no robot or mechatronic device was involved in the study [58,59]. A final list with 30 studies was identified as eligible for qualitative review. Among the 30 studies, 11 [60–70] were involved in testing the BCI-hand robot system on chronic and subacute stroke

medRxiv preprint doi: https://doi.org/10.1101/2019.12.11.19014571; this version posted December 15, 2019. The copyright holder for this preprint (which was not certified by peer review) is the author/funder, who has granted medRxiv a license to display the preprint in perpetuity.
It is made available under a CC-BY-NC-ND 4.0 International license .

patients ([60,65] are RCTs) while the rest involved testing on healthy participants [71–89]. Table 2 shows a summary of the relevant data fields extracted from these studies.

[Table 2 Around Here]

Technology Evaluation

EEG Acquisition

The choice of EEG system as well as the type of electrodes provides a technical trade-off and affects the session both in terms of subjective experiences (i.e., ease-of-use, preparation time, cleaning, comfortability) and data performance. Due to the presence of a conducting gel/solution, standard "wet" electrodes provide a degree of confidence in preventing signal disruption within a short duration usually enough for a standard stroke therapy session. However, this also makes the setup, use and cleaning in the experiment more challenging, non-ambulatory and reliant on a specialised laboratory setup [4]. Conversely, dry electrodes offer an accessible, user-friendly and portable alternative by using dry metal pins or coatings that comb through hair and come in contact directly with the scalp. The signal fidelity of dry electrodes is still a matter of debate in the BCI community. A systematic comparison between dry passively-amplified and wet actively-amplified electrodes reported similar performance in the detection of event-related potentials (ERP) [90]. However, for a study involving dry active electrodes [91], high inter-electrode impedance resulted in increased single-trial and average noise levels as compared to both active and passive wet electrodes. In classifying MI, movement-related artefacts adversely affect active dry electrodes, but these can be addressed through a hybrid system of other physiological sensors to separate sources [92].

medRxiv preprint doi: https://doi.org/10.1101/2019.12.11.19014571; this version posted December 15, 2019. The copyright holder for this preprint (which was not certified by peer review) is the author/funder, who has granted medRxiv a license to display the preprint in perpetuity.
It is made available under a CC-BY-NC-ND 4.0 International license .

The EEG acquisition systems involved in the studies ranged from low-cost devices having few electrode channels (2-15 gel or saline-soaked silver/silver chloride [Ag/AgCl] electrodes) to standard EEG caps that had higher spatial resolution (16-256 gel or saline-soaked Ag/AgCl electrodes). The placement of EEG channels was accounted for by studies involving MI (N=21). This allowed us to determine the usage frequency among electrodes and is presented in Figure 2 as a heat map generated in R Studio (using the packages: “akima”, “ggplot2” and “reshape2”) against the 10-20 international electrode placement system.

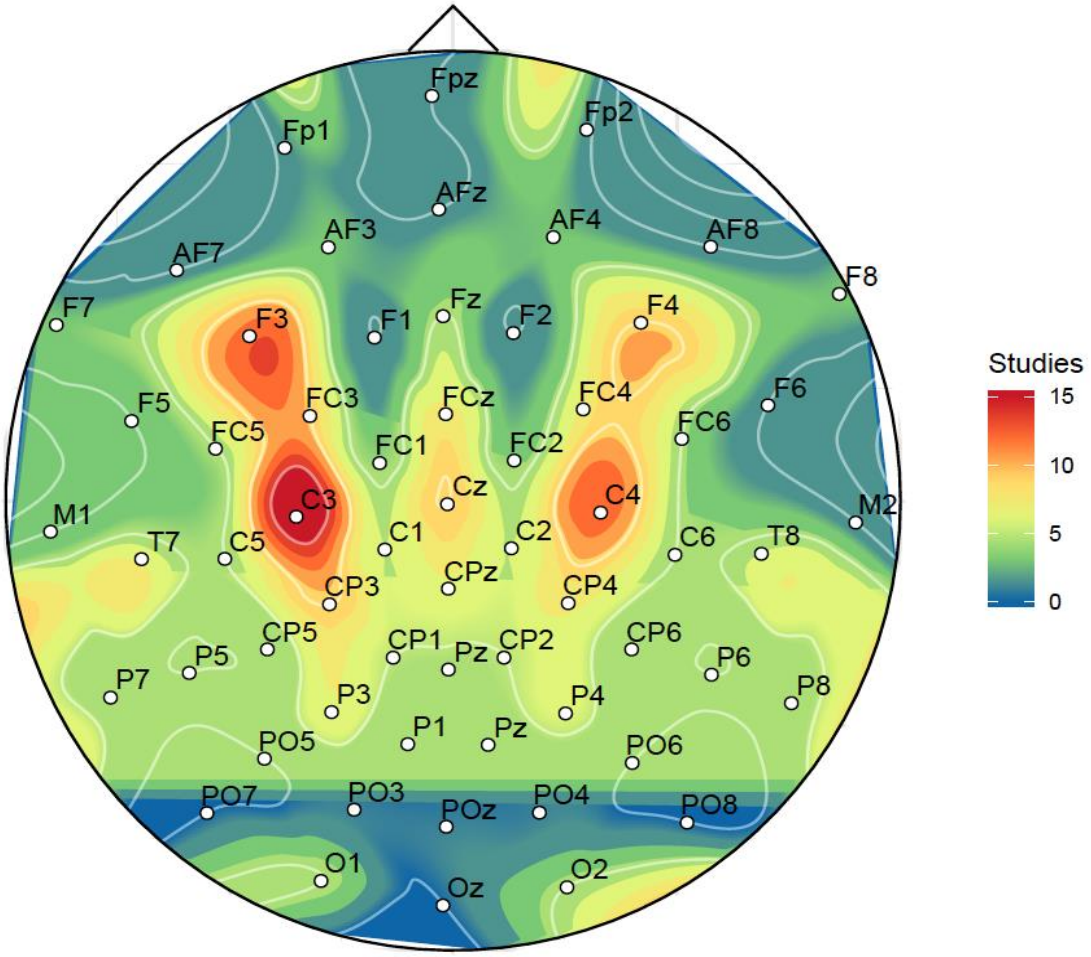

Figure 2. EEG Channel Usage across Motor Imagery Studies (N=21)

medRxiv preprint doi: https://doi.org/10.1101/2019.12.11.19014571; this version posted December 15, 2019. The copyright holder for this preprint (which was not certified by peer review) is the author/funder, who has granted medRxiv a license to display the preprint in perpetuity.
It is made available under a CC-BY-NC-ND 4.0 International license .

It can be seen that the EEG channels used for MI studies are concentrated towards electrodes along the central sulcus (C) region and the frontal lobe (F) region of the placement system where the motor cortex strip lies. Among these, C3 (N=17) and F3 (N=14) were mostly used, presumably because a majority of the participants were right-handed. The next most frequent were C4 (N=13) and the electrodes F4, Cz and CP3 (N=10).

Signal Processing: Feature Extraction and Classification

It is necessary to process EEG data if they are to be used as a control signal. First, the data need to undergo a series of pre-processing routines (e.g., filtering and artefact removal) before feature extraction and classification for use as a control signal for the robotic hand. Feature extraction involves recognising useful information (e.g., spectral power, time epochs, spatial filtering) for better discriminability among mental states. For example, the common spatial patterns (CSP) algorithm is a type of spatial filter that learns and maximises the variance of band pass-filtered EEG from one class to discriminate it to the other [93].

In the EEG-based BCI studies examined, it was found that the feature extraction and classification techniques were variable between systems. Table 3 provides a summary of pre-processing, feature extraction and classification techniques across the studies. There was a wide variation in the implemented signal processing strategies, but a unifying theme across studies was the attempt to: (i) discriminate mental states recorded in EEG across different manual tasks; (ii) classify the different states to produce a viable signal.

Table 3. BCI Feature Extraction and Classification

Study	Pre-Processing	Feature Extraction	Classification	Hand Task
Ang et al. [60]	Band-pass (0.05-40 Hz)	Filter Bank Common Spatial Pattern	Calibration model (unspecified)	MI vs rest

medRxiv preprint doi: https://doi.org/10.1101/2019.12.11.19014571; this version posted December 15, 2019. The copyright holder for this preprint (which was not certified by peer review) is the author/funder, who has granted medRxiv a license to display the preprint in perpetuity.
It is made available under a CC-BY-NC-ND 4.0 International license .

		(FBCSP) algorithm [94]		
Barsotti et al. [61]	Band-pass (8-24 Hz)	ERD (β and μ-decrease), CSP	SVM with linear kernel	MI vs rest
Bauer et al. [82]	Band-pass (6-16 Hz using zero-phase lag FIR	ERD (β-decrease)	Linear autoregressive model based on Burg Algorithm	MI vs rest
Bundy et al. [62]	Unspecified	ERD (β and μ-decrease)	Linear autoregressive model	MI (affected, unaffected) vs rest
Chowdhury et al. [63]	Band-pass (0.1 Hz-100 Hz), Notch (50 Hz)	CSP Covariance-based, ERD/ERS (β and μ-change)	SVM with linear kernel, Covariate Shift Detection (CSD)-based Adaptive Classifier	left vs right MI
Coffey et al. [77]	Band-pass (0.5 Hz-30 Hz), Notch (50 Hz)	CSP Covariance-based	Linear Discriminant Analysis (LDA) classifier	MI vs rest
Diab et al. [88]	Unspecified	Time epochs (unspecified)	Artificial Neural Network (ANN)-based Feed Forward Back Propagation	Non-MI open vs closed
Frolov al. [65]	Band-pass (5-30 Hz), FIR (order 101), IIR notch Chebyshev type I filter (50 Hz)	Time epochs (10 s)	Bayesian-based EEG covariance classifier [95]	MI (affected, unaffected) vs rest
Ono et al. [66]	Band-pass (0.5-30 Hz), notch (50 or 60 Hz)	Time epochs (700 ms), ERD (μ-decrease)	Linear Discriminant Analysis (LDA) classifier	MI vs rest
Ramos-Murguialday et al. [80]	Unspecified	Time epochs (5 s), Spatial filter, ERD/ERS (β and μ-change)	Linear autoregressive model	MI vs rest
Vukelic and Gharabaghi [84]	High-pass (unspecified)	ERD (β-decrease)	Linear autoregressive model based on Burg Algorithm	MI vs rest
Witkowski et al. [86]	Band-pass (0.4-70 Hz), Laplacian filter	ERD/ERS (β and μ-change)	Linear autoregressive model based on Yule-Walker algorithm	MI vs rest

SVM = Support Vector Machines, FIR = Finite Impulse Response, IIR = Infinite Impulse Response

medRxiv preprint doi: https://doi.org/10.1101/2019.12.11.19014571; this version posted December 15, 2019. The copyright holder for this preprint (which was not certified by peer review) is the author/funder, who has granted medRxiv a license to display the preprint in perpetuity.
It is made available under a CC-BY-NC-ND 4.0 International license .

Robot-Assisted Rehabilitation

Robotic hand rehabilitation systems provide kinaesthetic feedback to the user during BCI trials. Most of these devices are powered by either DC motors, servomotors or pneumatic actuators that transmit energy via rigid links or Bowden cables in a tendon-like fashion. The studies in this review included single-finger [69–71], multi-finger [67] (including EMOHEX [63,64,72]), full hand gloves [73,74] (including mano: Hand Exoskeleton [75] and Gloreha [76]) and full arm exoskeletons with isolated finger actuation (BRAVO-Hand [61]). Nine of the studies [62,72,73,75,77–81] presented their novel design of a hand rehabilitation device within the article while some reported on devices reported elsewhere (i.e., in a previous study of the group or a research collaborator). Two commercially-available devices were also used: AMADEO (Tyromotion, Austria) is an end-effector device used in 3 studies [82–84], and Gloreha (Idrogenet, Italy) is a full robotic hand glove used by Tacchino et al. [76]. AMADEO and Gloreha are both rehabilitation devices that have passed regulatory standards in their respective regions. AMADEO remains the gold standard for hand rehabilitation devices as it has passed safety and risk assessments and provided favourable rehabilitation outcomes. The International Classification of Functioning, Disability and Health (ICF) provides three specific domains that can be used to assess an intervention of this kind: improving impairments, supporting performance of activities and promoting participation [96,97]. In this case, a gold standard device not only prioritises user safety (established early in the development process) but also delivers favourable outcomes in scales against these domains. Figure 3 shows the main types of robotic hand rehabilitation devices.

medRxiv preprint doi: https://doi.org/10.1101/2019.12.11.19014571; this version posted December 15, 2019. The copyright holder for this preprint (which was not certified by peer review) is the author/funder, who has granted medRxiv a license to display the preprint in perpetuity.
It is made available under a CC-BY-NC-ND 4.0 International license .

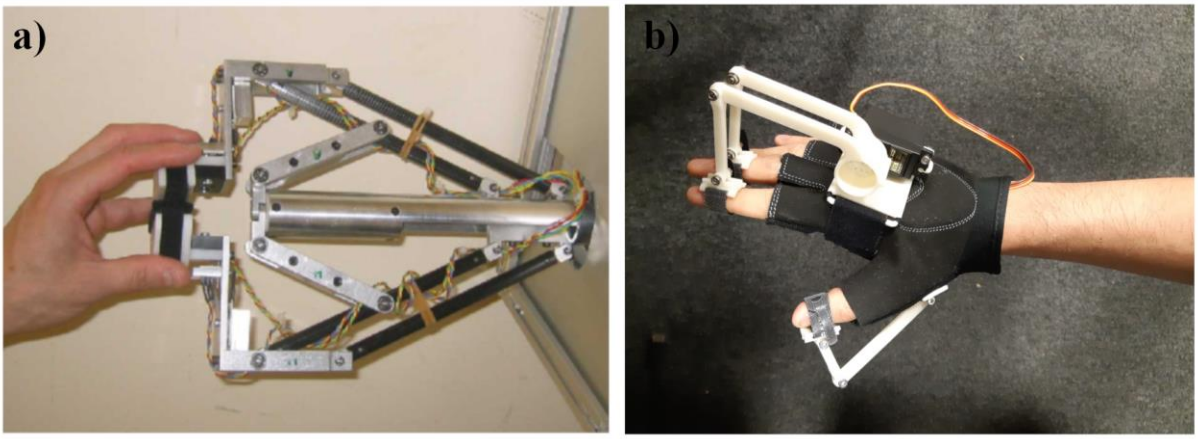

Figure 3. Robotic hand rehabilitation devices: a) An end-effector device (Haptic Knob) used in one of the extracted studies [60,98]**, b) a wearable hand exoskeleton/orthosis**

Quality Assessment

A Technology Readiness Assessment (TRA) was performed for each study and the Technology Readiness Levels (TRL) are presented in Table 4. While some of the system components (especially among robotic devices) were commercially available (having TRL 9+), we performed a TRA on the whole system (the interaction between BCI and robotics) to provide an evaluation of its maturity and state-of-the-art development with regard to rehabilitation medicine. We further assessed the TRL of each system at the time of the publication and its subsequent development.

Table 4. Technology Readiness Assessment of the BCI-Hand Robot Systems

Levels	Description	Studies
TRL 1	• Lowest level of technological readiness • Literature reviews and initial market surveys • Scientific application to defined problems	
TRL 2	• Generation of hypotheses • Development of research plans and/or protocols	

medRxiv preprint doi: https://doi.org/10.1101/2019.12.11.19014571; this version posted December 15, 2019. The copyright holder for this preprint (which was not certified by peer review) is the author/funder, who has granted medRxiv a license to display the preprint in perpetuity.
It is made available under a CC-BY-NC-ND 4.0 International license .

TRL 3	• Testing of hypotheses – basic research, data collection and analysis • Testing of design/prototype – verification and critical component specifications • Initial proof-of-concept in limited amount of laboratory/animal models	Most studies from the prototype group (N=18) [71–87,89]
TRL 4	• Proof-of-concept of device/system in defined laboratory/animal models • Safety testing – problems, adverse events and potential side effects	Witkowski et al., 2014 [88]
TRL 5	• Comparison of device/system to other existing modalities or equivalent devices/systems • Further development – testing through simulation (tissue or organ models), animal testing • Drafting of Product Development Plan	Barsotti et al., 2015 [61], Ono et al., 2016 [66], Chowdhury et al., 2018-b [63], Tsuchimoto et al., 2019 [69]
TRL 6	• Small scale clinical trials (Phase 1) – under carefully controlled and intensely monitored clinical conditions	Carino-Escobar et al., 2019 [70], Chowdhury et al., 2018-c [64], Norman et al., 2018 [67], Wang et al., 2018 [68]
TRL 7	• Clinical trials (Phase 2) – safety and effectiveness integration in operational environment	Ang et al., 2014 [60], Frolov et al., 2017 [65]
TRL 8	• Clinical trials (Phase 3) – evaluation of overall risk-benefit of device/system use • Confirmation of QSR compliance • Awarding of PMA for device/system by CDRH or equivalent agency	
TRL 9	• The device/system may be distributed/marketed	

QSR = Quality System Requirements, PMA = Premarket Approval, CDRH = Center for Devices and Radiological Health

medRxiv preprint doi: https://doi.org/10.1101/2019.12.11.19014571; this version posted December 15, 2019. The copyright holder for this preprint (which was not certified by peer review) is the author/funder, who has granted medRxiv a license to display the preprint in perpetuity.
It is made available under a CC-BY-NC-ND 4.0 International license .

Clinical Evaluation

Studies with Stroke Patients (Clinical Group)

A total of 208 stroke patients (with sample size varying 3-74) were involved in the 11 clinical studies. One study [60] reported a 3-armed RCT with control groups as device-only and SAT while another study [65] was a multi-centre RCT with sham as the control group. Five studies were uncontrolled – where the aims were either to study classification accuracies during sessions [61], to monitor clinical outcomes improvement from Day 0 until the end of the programme [62,70] or both [64,67]. Two studies [68,69] compared effects of the intervention against SHAM feedback. Another study [63] compared the classification accuracies of healthy and hemiplegic stroke patients against two BCI classifiers while the remaining study [66] compared classification accuracies from stroke patients who receive congruent or incongruent visual and kinaesthetic feedback.

Most of the studies adopted FMMA, ARAT and GS measurements to assess clinical outcomes. Six studies [60,62,64,65,68,70] reported patient improvement in these measures when subjected to BCI-hand robot interventions; in contrast with their respective controls or as recorded through time in the programme. For Ang et al. [60], FMMA Distal scores were reported in weeks 3, 6, 12 and 24 and the BCI-device group (N=6) yielded the highest improvement in scores across all time points as compared to the device only (N=8) and SAT (N=7) groups. Bundy et al. [62] reported an average of 6.20±3.81 improvement in the ARAT scores of its participants (N=10) in the span of 12 weeks while Chowdhury et al. [64] reported a group mean difference of +6.38 kg ($p=0.06$) and +5.66 ($p<0.05$) in GS and ARAT scores, respectively (N=4). Frolov et al.'s [65] multi-centre RCT reported a higher improvement in the FMMA Distal, ARAT Grasp and ARAT Pinch scores of the BCI-device group (N=55) when compared to the control/SHAM group (N=19), but not in the ARAT Grip

medRxiv preprint doi: https://doi.org/10.1101/2019.12.11.19014571; this version posted December 15, 2019. The copyright holder for this preprint (which was not certified by peer review) is the author/funder, who has granted medRxiv a license to display the preprint in perpetuity.
It is made available under a CC-BY-NC-ND 4.0 International license .

scores where the values are both equal to 1.0 with $p<0.01$ for the BCI-device group and $p=0.045$ for the control.

Studies with Healthy Participants (Prototype Group)

The studies which involved pilot testing on healthy human participants had a combined total of individuals (sample size ranging from 1-32) who had no history of stroke or other neurological diseases. Right-handed individuals made up 44.24% of the combined population while the other 55.76% were unreported. These studies aimed to report the successful implementation of a BCI-robot system for hand rehabilitation and were more heterogeneous in terms of study and task designs than those studies that involved clinical testing. The most common approach was to design and implement a hand orthosis controlled by MI which accounted for 9 out of the 19 studies and were measured based on classification accuracy during the calibration/training period and online testing. Li et al. [73] and Stan et al. [79] also aimed to trigger a hand orthosis but instead of MI, the triggers used by Li et al. is based on an attention threshold while Stan et al. used a vision-based P300 speller BCI. Bauer et al. [82] compared MI against ME using a BCI-device while Ono et al. [85] studied the implementation of an action observation strategy with a combined visual and kinaesthetic feedback or auditory feedback. Five more studies [76,80,81,83,84] focused on varying the feedback while two more [74,86] assessed the performance and safety of a hybrid BCI with EMG, EOG or both.

For the studies that had a clinical testing component, a methodological quality assessment by the PEDro Scale was performed. Two studies which appeared on the PEDro search [60,65] had predetermined scores in the scale and were extracted for this part while the rest were manually evaluated by the authors. Table 5 shows the results of the methodological quality

medRxiv preprint doi: https://doi.org/10.1101/2019.12.11.19014571; this version posted December 15, 2019. The copyright holder for this preprint (which was not certified by peer review) is the author/funder, who has granted medRxiv a license to display the preprint in perpetuity.
It is made available under a CC-BY-NC-ND 4.0 International license .

assessment against the scale. Note that in the PEDro Scale, the presence of an eligibility criteria is not included in the final score.

Table 5. Methodological Quality of Clinical Studies based on PEDro Scale

	Criteria	**Ang et al.**	**Barsotti et al.**	**Bundy et al.**	**Carino-Escobar et al.**	**Chowdhury-b**	**Chowdhury-c**	**Frolov et al.**	**Norman et al.**	**Ono et al.**	**Tsuchimoto et al.**	**Wang et al.**
1	Eligibility criteria*	1	1	1	1	1	1	1	1	0	1	1
2	Random allocation	1	0	0	0	0	0	1	0	0	1	1
3	Concealed allocation	0	0	0	0	0	0	0	0	0	1	1
4	Baseline comparability	1	0	1	0	1	1	1	0	0	0	0
5	Blind subjects	0	0	0	0	0	0	0	0	0	1	1
6	Blind therapists	0	0	0	0	0	0	0	0	0	1	0
7	Blind assessors	1	0	0	0	0	0	1	0	0	0	1
8	Adequate follow-up	1	1	1	1	1	1	0	1	1	1	1
9	Intention-to-treat analysis	0	0	1	1	1	1	0	1	0	0	0
10	Between-group comparisons	1	0	0	0	1	0	1	0	1	1	1
11	Point estimates and variability	1	1	1	1	1	0	1	1	1	1	1
Total		**6**	**2**	**4**	**4**	**5**	**3**	**5**	**4**	**3**	**7**	**7**

*not included in the final score

medRxiv preprint doi: https://doi.org/10.1101/2019.12.11.19014571; this version posted December 15, 2019. The copyright holder for this preprint (which was not certified by peer review) is the author/funder, who has granted medRxiv a license to display the preprint in perpetuity.
It is made available under a CC-BY-NC-ND 4.0 International license .

Discussion

To the best of our knowledge, this article was the first to compile BCI-driven robotic systems specific for hand rehabilitation. During this review, we found several limitations present among the studies collected and we examine these in more detail here and provide recommendations for future work in this area.

To provide clarity on the state-of-the-art and development of BCI-hand robot systems, we looked into the maturity of technology used in each study and determined by its readiness level (TRL). All but one in the prototype group was rated as having TRL 3 while the clinical group was more varied in their TRL (ranging from 5-7). The system used by Witkowski et al. [86], a prototype study, was rated TRL 4 due to the study being performed on the basis of improving and assessing its safety features. It is also worth noting that while a formal safety assessment was not performed for the TRL 3 prototypes of Stan et al. [79], Randazzo et al. [75] and Tacchino et al. [76], safety considerations and/or implementations were made; a criterion to be satisfied before proceeding to TRL 4. The system used by Chowdhury et al. is a good example of improving a TRL from 5 to 6 with a pilot clinical study published within the same year [63,64]. The two systems used in the RCT studies by Ang et al. [60] and Frolov et al. [65] achieved the highest score (TRL 7) among all of the studies which also meant that no BCI-hand robot system for stroke rehabilitation has ever been registered and commercially-released to date. This suggests that such systems lack the strong evidence that would propel commercialisation and technology adoption.

Heterogeneity in the study designs was apparent in both the clinical and prototype groups. The lack of control groups and random allocation in clinical studies (e.g., only 2 out of 7 studies are in the huge sample size RCT stage) made us unable to perform a meta-analysis of

medRxiv preprint doi: https://doi.org/10.1101/2019.12.11.19014571; this version posted December 15, 2019. The copyright holder for this preprint (which was not certified by peer review) is the author/funder, who has granted medRxiv a license to display the preprint in perpetuity.
It is made available under a CC-BY-NC-ND 4.0 International license .

effects and continue the study by Cervera et al [36] with a focus on BCI-hand robot interventions. Results from the methodological quality assessment showed that only two studies [68,69] had a score of 7 in the PEDro scale. Although non-conclusive, these results support the notion that most of the studies are not aligned with the criteria of high-quality evidence-based interventions. These factors also raise the need to develop clearly defined protocols when conducting BCI-hand robot studies on stroke patients. Until new systems have been assessed on this standard, it will be difficult to generate strong evidence supporting the effectiveness of BCI-robotic devices for hand rehabilitation.

In the development of any BCI-robotic device there are several design and feature considerations that need to be made to ensure that the systems are both fit for purpose and acceptable to the end-user. These design considerations must go beyond the scope of understanding the anatomy of the hand and the physiology of motor recovery in response to therapy. Feedback from stroke patients should be an essential part of this design process. the extracted studies, we surveyed the extent of end-user involvement in the initial stages of development (i.e., through consultations, interviews and therapy observations) and we found that there were no explicit statements about these in the reports. We recommend, as good practice, for future work in this area to report the type and degree of patient and/or physician involvement in device development to allow reviewers and readers to more readily gauge the potential usability of the system.

We were able to profile the BCI-hand robot systems regarding their technical specifications and design features. In hardware terms, a BCI-hand robot system involves three major components: (1) An EEG data acquisition system with several electrodes connected to a signal amplifier; (2) A computer where raw EEG data is received then processed by filters

medRxiv preprint doi: https://doi.org/10.1101/2019.12.11.19014571; this version posted December 15, 2019. The copyright holder for this preprint (which was not certified by peer review) is the author/funder, who has granted medRxiv a license to display the preprint in perpetuity.
It is made available under a CC-BY-NC-ND 4.0 International license .

and classifiers and where most of the cues and feedback during training is presented via a visual display; (3) a robotic hand rehabilitation system for providing the physical therapy back to the user.

The majority of the studies (N=19) used a BCI solely based on EEG while the rest were combined with other sensors: EEG with EMG [60,63,72,76,80–83], EEG with force sensors [64] and an EEG-EMG-EOG hybrid system [74,86]. The purpose of this integration is mainly to improve signal quality by accounting for artefacts or to provide added modalities. Action potentials such as those caused by ocular and facial movements interfere with nearby electrodes and the presence of an added electrophysiological sensor accounting for these would enable the technician to perform noise cancellation techniques as a first step in signal processing. Almost all of the studies included used a standard EEG system with "wet" electrodes (e.g., g.USBamp by g.tec and BrainAmp by Brain Products) while three used Emotiv EPOC+, a semi-dry EEG system that uses sponge conductors infused with saline solution. While the use of dry electrodes has been observed in pilot and prototype studies of BCI-hand robot systems [52,49,78,87] and other motor imagery experiments [99–102], no dry EEG system was used in the final 30 studies that tested healthy or stroke participants. It is expected that as dry EEG systems continue to improve, their use in clinical studies of BCI will also become increasingly prominent.

The degree of BCI-robotic control for the majority of the studies (N=26) was limited to triggering the device to perform grasping (opening and closing of hand) and pinching (a thumb-index finger pinch or a 3-point thumb-index-middle finger pinch) movements using MI and other techniques. This means that no robotic control setup among the screened studies were able to perform digit-specific MI. This is a limitation caused by the non-invasive setup

medRxiv preprint doi: https://doi.org/10.1101/2019.12.11.19014571; this version posted December 15, 2019. The copyright holder for this preprint (which was not certified by peer review) is the author/funder, who has granted medRxiv a license to display the preprint in perpetuity.
It is made available under a CC-BY-NC-ND 4.0 International license .

of EEG and is due to the low spatial resolution brought by the distances between electrodes [103]. The homunculus model, a representation of the human body in the motor strip, maps the areas of the brain where activations have been reported to occur for motor processes. The challenge of decoding each finger digit MI in one hand is that they only tend to occupy a small area in this strip. Hence even the highest resolution electrode placement system (i.e., the five percent or 10-5 system – up to 345 electrodes) would have difficulties accounting for digit-specific MI for BCI. In contrast to EEG, electrocorticography (ECoG) have been used to detect digit-specific MI. The electrodes of ECoG come in contact directly with the motor cortex and is an invasive procedure; making it non-ideal for use in BCI therapy [104]. It is worth noting however that some studies were successful in implementing continuous control based on ERD/ERS patterns: Bundy et al. [62] and Norman et al. [67] were able to apply continuous control of a 3-DOF pinch-grip exoskeleton based on spectral power while Bauer et al. [82] provided ERD-dependent control of finger extension for an end-effector robot. These continuous control strategies have been shown to be very useful in BCI-hand robots for assistive applications (i.e., partial or full device dependence for performing ADL tasks [105]). Whether this type of control can significantly improve stroke recovery is still in question as the strategy of robots for stroke rehabilitation can be more classified as a therapeutic "exercise" device.

Signal processing and machine learning play a vital role in the development of any EEG-based BCI. The pre-processing techniques (e.g., filtering, artefact removal), types of features computed from EEG, and the classifier used in machine learning can significantly affect the performance of the robotic system in classifying the user's intent via MI [106]. This systematic review has revealed that approaches to develop MI EEG-based BCI are highly diverse in nature, which makes it difficult to compare across the systems and hinders the

medRxiv preprint doi: https://doi.org/10.1101/2019.12.11.19014571; this version posted December 15, 2019. The copyright holder for this preprint (which was not certified by peer review) is the author/funder, who has granted medRxiv a license to display the preprint in perpetuity.
It is made available under a CC-BY-NC-ND 4.0 International license .

development of new BCI systems informed by the strengths and weaknesses of existing state-of-the-art systems. The diversity in the design process can be beneficial to develop complex MI EEG-based BCI systems to achieve high efficiency and efficacy. However, such newly developed systems should be open sourced and easily reproducible by the research community to provide valid performance comparisons and drive forward the domain of robotic-assisted rehabilitation.

In addition to MI, other strategies for robotic control were reported. Diab et al. [88] and King et al. [89] both facilitated the movements of their respective orthoses by physical practice while Stan et al. [79] utilised a P-300 evoked potential speller BCI, where the user visually focused on a single alphanumerical character situated in a grid. The chosen character then corresponded to a command for the hand orthosis thereby producing the desired stimulus for the patient. While the latter study reported 100% accuracy rate in terms of intention and execution, the EEG channels were situated in the visual cortex rather than the motor strip which deviates from the goal of stimulating the desired brain region for plasticity.

In order to facilitate hand MI and account for significant time-points in the EEG data, all the studies employed a cue-feedback strategy during their trials. 19 of the studies presented a form of visual cue while the rest, except for two unspecified [69,87], involved cues in auditory ("bleep") [76,80–83], textual [78,79,89] or verbal [88] forms. As for the provision of a matching sensory feedback, 16 studies presented a combination of kinaesthetic and visual feedback with some also providing auditory feedback during successful movement attempts. All the studies provided kinaesthetic feedback through their robotic devices. Some systems with visual feedback, such as Wang et al. [68], Li et al. [73], Chowdhury et al. in both of their clinical studies [63,64] and Ono et al. in their clinical [66] and pilot testing experiments [85],

medRxiv preprint doi: https://doi.org/10.1101/2019.12.11.19014571; this version posted December 15, 2019. The copyright holder for this preprint (which was not certified by peer review) is the author/funder, who has granted medRxiv a license to display the preprint in perpetuity.
It is made available under a CC-BY-NC-ND 4.0 International license .

used a video of an actual hand performing the desired action. Ang et al. [60] and Stan et al. [79], in a different strategy, provided visual feedback through photo manipulation and textual display, respectively. While the latter two studies reported promising results (with Ang et al. in RCT stage and Stan et al. having 100% classification accuracy), it should also be considered that such cue and feedback types (including Graz visualisations and auditory forms) are non-representative of hand movement and may not provide the same stimulation as a geometrical representation of a hand moving its desired course. This may be essential when we base principles of stroke recovery in alignment with how MI correlates with AO – an underlying theme of the motor simulation theory proposed by Jeannerod [15]. Figure 4 shows how different kinds of visual cue and feedback can be presented to participants to help facilitate MI.

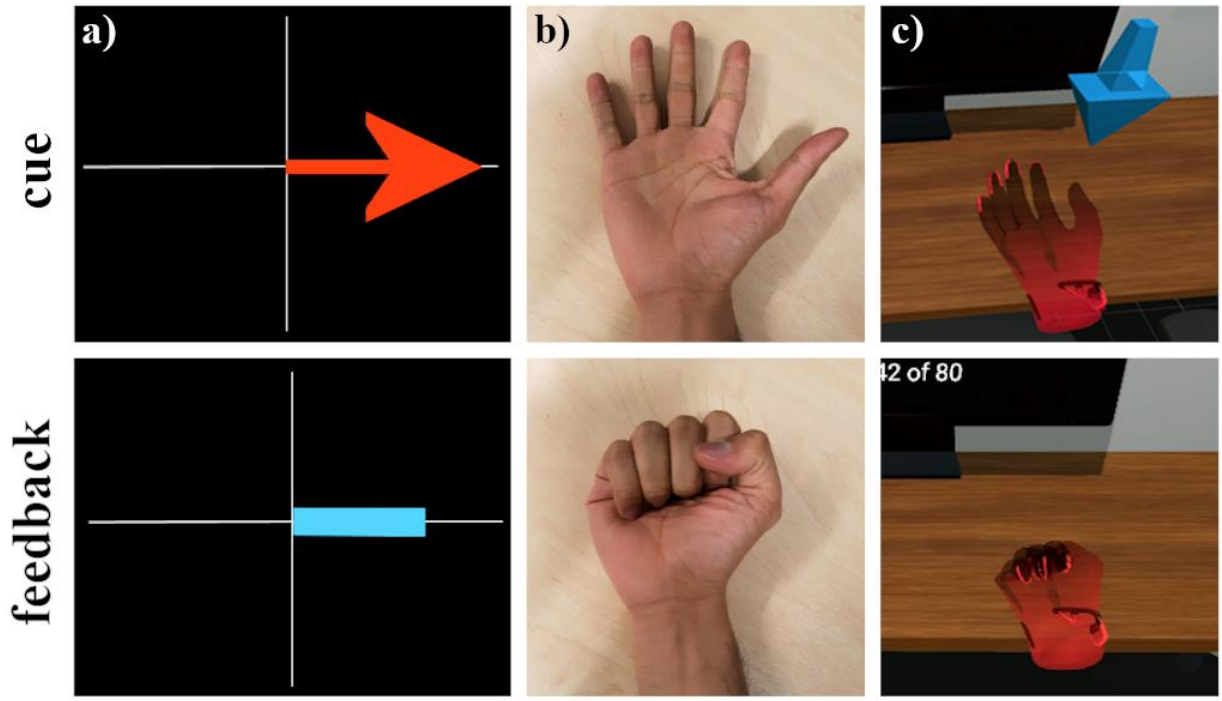

Figure 4. Visual cue and feedback during MI trials in different conditions. (a) Graz MI visualisations, (b) video recordings of hand movement and (c) virtual hand representation through VR/AR

medRxiv preprint doi: https://doi.org/10.1101/2019.12.11.19014571; this version posted December 15, 2019. The copyright holder for this preprint (which was not certified by peer review) is the author/funder, who has granted medRxiv a license to display the preprint in perpetuity.
It is made available under a CC-BY-NC-ND 4.0 International license .

Future Directions

There is clearly great potential for the use of BCI-hand robots in the rehabilitation of an affected hand following stroke. Nevertheless, it is important to emphasise that there is currently no solid evidence to support the use of such systems within clinical settings. Moreover, the purported benefits of these systems rest on conjectures that require empirical evidence. In other words, there are grounds for supposing that MI could be useful within these rehabilitation settings but no supporting evidence. This systematic review has also revealed that there are a number of technological limitations to existing BCI-hand robotic systems. We stress an urgent need to address these limitations to ensure that the systems meet the minimum required levels of product specification (in measuring brain activity, processing signals, delivering forces to the hand and providing rich feedback and motivating settings). We question the ethics or usefulness of conducting clinical trials with such systems until they can demonstrate minimum levels of technological capability. We consider below what standards these systems should obtain before subjecting them to a clinical trial and discuss might constitute an acceptable standard for a clinical trial.

Ideal Setup for a BCI-hand Robot

We summarise the information revealed via the systematic review about what constitutes an acceptable setup for a BCI-hand robot for stroke rehabilitation. We focus on improving individual components in data acquisition, data processing, the hand rehabilitation robot, and the visual cue and feedback environment. Table 6 presents the features and specifications of a fully integrated acceptable system.

medRxiv preprint doi: https://doi.org/10.1101/2019.12.11.19014571; this version posted December 15, 2019. The copyright holder for this preprint (which was not certified by peer review) is the author/funder, who has granted medRxiv a license to display the preprint in perpetuity.
It is made available under a CC-BY-NC-ND 4.0 International license .

Table 6. Exemplary Features and Specifications of Future BCI-Hand Robot Systems

Component	Features and Specifications
Data Acquisition System and Software	• Dry EEG system with 8-16 channels, comfortable and easy to use • Inclusion of other bio-signal sensors such as EMG, EOG, force, accelerometers to remove artefacts and improve classification • Robust and reliable signal processing software: machine learning-based algorithms that discriminate brain states such as MI or evoked potentials and have lower calibration times
Hand Robot	• Safe, comfortable and aligned with the hand's range of motion • Effective in providing kinaesthetic feedback • Use of back-drivable or soft actuators that effectively assist movement without additional injury • Multiple levels of safety and emergency features (mechanical, electronic, software), clear and obvious operation
Visual Cue and Feedback	• Provide rich visual cue and feedback to intended tasks, geometric representation of the hand (video or simulated environment), can be in multiple platforms such as display monitors or VR/AR headsets • Gamification of therapy exercises to provide an engaging regime to stroke patients

The implementation of these features in an ideal BCI-robot setup needs to be weighed against socioeconomic factors in healthcare delivery for it to be considered market ready. An ideal BCI system should provide above chance-level classification (>60%) after the first session on the first day of therapy. Ideally, the classification algorithm should also translate to following sessions or days; reducing the number of training sessions and focusing on the main therapy tasks. An alternative approach is to focus on making the setup an engaging experience. In other words, the delivery of intervention can be started immediately the patient wears the EEG cap and runs the BCI system. For the hand robot system, more straightforward criteria

medRxiv preprint doi: https://doi.org/10.1101/2019.12.11.19014571; this version posted December 15, 2019. The copyright holder for this preprint (which was not certified by peer review) is the author/funder, who has granted medRxiv a license to display the preprint in perpetuity.
It is made available under a CC-BY-NC-ND 4.0 International license .

can be followed with the existence of the numerous design protocols, regulation standards and assessment matrices mentioned in this review. Nevertheless, end-user involvement in the design with the prioritisation of safety while allowing the most natural hand movement and ROM as possible is the recommended goal.

Ideal Setup for Clinical Trials

We also propose a set of specialised criteria for BCI-hand robot systems in addition to the standard motor improvement scores (e.g. ARAT, FMMA) evaluated during clinical trials. Firstly, classification accuracies between intended and interpreted actions from the data acquisition and software component should always be accounted to track the effectiveness of BCI in executing the clinical task. In addition to this, system calibration and training procedures, especially its duration, should be detailed in the protocol to document the reliability of the classification algorithm. There is not much to consider in the use of robotic devices as they are most likely to be mature (if not yet commercially available) before being used as the hardware component in the study. However, the devices' functionality (i.e., task to be performed, degree of control and motion, actuation and power transmission etc.) should always be stated as they contribute to the evaluation of interactions between other components in the system. Lastly, controls for the clinical study must always be included, even with small-scale patient studies. As discussed in this article, these controls may be in the form of sham, standard arm therapy (SAT), standard robotic therapy, congruency feedback and quality of stimuli among others. Having regarded and implemented these criteria would help homogenise the clinical data for future meta-analyses, strengthen evidence-based results and provide a reliable way of documentation for individual and/or interacting components.

medRxiv preprint doi: https://doi.org/10.1101/2019.12.11.19014571; this version posted December 15, 2019. The copyright holder for this preprint (which was not certified by peer review) is the author/funder, who has granted medRxiv a license to display the preprint in perpetuity.
It is made available under a CC-BY-NC-ND 4.0 International license .

Proposed roadmap

We suggest that the immediate focus for BCI-controlled robotic device research should be around the engineering challenges. It is only when these challenges have been met that it is useful and ethical to subject the systems to clinical trials. We recommend that the challenges be broken down into the following elements: (1) data acquisition; (2) signal processing and classification; (3) robotic device; (4) priming and feedback environment; (5) integration of these four elements. The nature of these challenges means that a multidisciplinary approach is required (e.g. the inclusion of psychologists, cognitive neuroscientists and physiologists to drive the adoption of reliable neural data acquisition). It seems probable that progress will be made by different laboratories tackling some or all of these elements and coordinating information sharing and technology improvements. Once the challenges have been met (i.e. there is a system that is able to take neural signals and use these to help drive a robotic system capable of providing appropriate forces to the hand within a motivating environment) then robust clinical trials can be conducted to ensure that the promise of this approach does translate into solid empirical evidence supporting the use of these systems within clinical settings.

medRxiv preprint doi: https://doi.org/10.1101/2019.12.11.19014571; this version posted December 15, 2019. The copyright holder for this preprint (which was not certified by peer review) is the author/funder, who has granted medRxiv a license to display the preprint in perpetuity.
It is made available under a CC-BY-NC-ND 4.0 International license .

Conclusions

Research on BCI-controlled robotic devices for hand rehabilitation after stroke is a rapidly growing field and is gaining traction in the academic and medical research communities. The three main objectives of this systematic review were: (1) to survey how BCI technologies are utilised in controlling robotic devices for hand rehabilitation, (2) to determine the state-of-the-art developments in BCI systems in terms of hand MI resolution and degree of robotic control, and (3) to assess the clinical significance of BCI-hand robot systems by accounting clinical studies with outcome measures relating to motor recovery. Here, we were able to address these three and provide insight on the future of BCI-controlled robotics for stroke therapy.

We surveyed 30 EEG-based BCI-hand robot systems designed for stroke with majority of the studies (N=19) in their prototype development and pilot testing stages having TRL scores of 3-4. The rest of the studies (N=11) involved a clinical component into it, having tested on stroke patients. The systems used in the clinical group were rated with the highest technological readiness: TRL 7 for two studies undergoing RCT. Profiling the EEG acquisition systems confirmed the still dominance of standard EEG systems that uses “wet” electrodes over the recent dry electrode systems. However, as the latter’s technology continues to improve in the next years, we may see a positive shift towards these techniques in terms of usage and preference. The common goal among these studies is to successfully discriminate and with high accuracy a user’s intent via motor imagery. While most have reported reliable, above chance-level accuracy rates, we observe the limitations evident in hand motor imagery resolution (e.g., intention to grasp or pinch as opposed to rest, discriminating from left and right movement, signal processing techniques) and the degree of robotic control (i.e., triggering and continuous control). The task designs, cues and matching

medRxiv preprint doi: https://doi.org/10.1101/2019.12.11.19014571; this version posted December 15, 2019. The copyright holder for this preprint (which was not certified by peer review) is the author/funder, who has granted medRxiv a license to display the preprint in perpetuity.
It is made available under a CC-BY-NC-ND 4.0 International license .

sensory feedback modes play an important role in motor imagery ability. We give attention to the inferior visual stimuli presented in most of the trials and suggest the use of a rich and engaging one through the different immersive platforms such as Virtual Reality and Augmented Reality. We also report that the clinical adoption of BCI-hand robots is still in its infancy due to few studies reporting significant improvements in the functional recovery of stroke patients. We suggest the development of a standard protocol in assessing clinical outcomes as an effort to strengthen the argument that these systems are not only economically feasible but also viable and robust for the therapy of motor impairment post-stroke.

Finally, we recommend that future developers focus on end-user involvement in the early design stages, achieving the successful integration of the individual components and making the system as safe and cost-effective as possible without compromising on reliability and robustness. These steps should allow this promising technology to advance, be adopted by the stakeholders and improve the quality of life for stroke survivors.

medRxiv preprint doi: https://doi.org/10.1101/2019.12.11.19014571; this version posted December 15, 2019. The copyright holder for this preprint (which was not certified by peer review) is the author/funder, who has granted medRxiv a license to display the preprint in perpetuity.
It is made available under a CC-BY-NC-ND 4.0 International license .

List of Abbreviations

ADL	Activities of Daily Living
ANN	Artificial Neural Network
AO	Action Observation
AR	Augmented Reality
ARAT	Action Research Arm Test
BCI	Brain-Computer Interface
BMI	Brain-Machine Interface
CDRH	Center for Devices and Radiological Health
CSD	Covariate Shift Detection
CSP	Common Spatial Pattern
DC	Direct Current
ECoG	Electrocorticography
EEG	Electroencephalography
EMG	Electromyography
EOG	Electrooculography
ERD	Event-Related Desynchronisation
ERP	Event-Related Potential
ERS	Event-Related Synchronisation
ERSP	Event-Related Spectral Perturbation
FBCSP	Filter Bank Common Spatial Pattern
FIR	Finite Impulse Response
FMMA	Fugl-Meyer Motor Assessment
GS	Grip Strength
IIR	Infinite Impulse Response

medRxiv preprint doi: https://doi.org/10.1101/2019.12.11.19014571; this version posted December 15, 2019. The copyright holder for this preprint (which was not certified by peer review) is the author/funder, who has granted medRxiv a license to display the preprint in perpetuity.
It is made available under a CC-BY-NC-ND 4.0 International license .

LDA	Linear Discriminant Analysis
ME	Motor Execution
MI	Motor Imagery
PEDro	Physiotherapy Evidence Database
PMA	Premarket Approval
PRISMA	Preferred Reporting Items for Systematic Reviews and Meta-Analysis
PROSPERO	International Prospective Register of Systematic Reviews
PS	Pinch Strength
QSR	Quality System Requirement
RCT	Randomised Clinical Trial
SAT	Standard Arm Therapy
SVM	Support Vector Machine
TRA	Technology Readiness Assessment
TRL	Technology Readiness Levels
UK-MRC	United Kingdom Medical Research Council
VR	Virtual Reality

medRxiv preprint doi: https://doi.org/10.1101/2019.12.11.19014571; this version posted December 15, 2019. The copyright holder for this preprint (which was not certified by peer review) is the author/funder, who has granted medRxiv a license to display the preprint in perpetuity.
It is made available under a CC-BY-NC-ND 4.0 International license .

Declarations

Funding

This work was supported by a Newton Fund PhD grant, ID 331486777, under the Newton-Agham partnership. The grant is funded by the UK Department for Business, Energy and Industrial Strategy and the Philippine Commission on Higher Education and delivered by the British Council. For further information, please visit www.newtonfund.ac.uk.

Availability of Data and Materials

A full database of selected studies including those extracted during the search and selection process is available from the corresponding author on reasonable request.

Authors' Contributions

PDEB and ECS performed the initial search and screening of the studies. MA performed the analysis of signal processing techniques. AA, AEJ and RJH made contribution to the robotics, design and other engineering aspects of the current work. FM provided analysis related to EEG and BCI. MMW contributed to the clinical and overall direction of the review. PDEB, FM and MMW were the major contributors to the writing of the manuscript. All authors read and approved the final manuscript.

Competing Interests

The authors declare that they have no competing interests.

Ethics Approval and Consent to Participate

Not applicable.

medRxiv preprint doi: https://doi.org/10.1101/2019.12.11.19014571; this version posted December 15, 2019. The copyright holder for this preprint **(which was not certified by peer review)** is the author/funder, who has granted medRxiv a license to display the preprint in perpetuity.
It is made available under a CC-BY-NC-ND 4.0 International license .

Consent for Publication

Not applicable.

Acknowledgements

Not applicable.

medRxiv preprint doi: https://doi.org/10.1101/2019.12.11.19014571; this version posted December 15, 2019. The copyright holder for this preprint (which was not certified by peer review) is the author/funder, who has granted medRxiv a license to display the preprint in perpetuity.
It is made available under a CC-BY-NC-ND 4.0 International license .

References

1. McHugh G, Swain ID. A comparison between reported therapy staffing levels and the department of health therapy staffing guidelines for stroke rehabilitation: a national survey. BMC Health Services Research. 2014;14:216.

2. Ntsiea MV. Current stroke rehabilitation services and physiotherapy research in South Africa. S Afr J Physiother. 2019;75:475–475.

3. Manguerra MV, Baniqued PDE, Abad AC, Baldovino RG, Dungao JR, Bugtai NT. Active motor control for an upper extremity exoskeleton. Advanced Science Letters. 2018;24:9937–8840.

4. Graimann B, Allison B, Pfurtscheller G. Brain–computer interfaces: a gentle introduction. In: Graimann B, Pfurtscheller G, Allison B, editors. Brain-Computer Interfaces: Revolutionizing Human-Computer Interaction [Internet]. Berlin, Heidelberg: Springer Berlin Heidelberg; 2010. p. 1–27. Available from: https://doi.org/10.1007/978-3-642-02091-9_1

5. Chang WH, Kim YH. Robot-assisted therapy in stroke rehabilitation. Journal of stroke. 2013;15:174–81.

6. Jackson AE, Levesley MC, Makower SG, Cozens JA, Bhakta BB. Development of the iPAM MkII system and description of a randomized control trial with acute stroke patients. 2013 IEEE 13th International Conference on Rehabilitation Robotics (ICORR). 2013. p. 1–6.

7. Hochberg LR, Serruya MD, Friehs GM, Mukand JA, Saleh M, Caplan AH, et al. Neuronal ensemble control of prosthetic devices by a human with tetraplegia. Nature. 2006;442:164.

8. Silvoni S, Ramos-Murguialday A, Cavinato M, Volpato C, Cisotto G, Turolla A, et al. Brain-computer interface in stroke: a review of progress. Clin EEG Neurosci. 2011;42:245–52.

9. Molteni F, Gasperini G, Cannaviello G, Guanziroli E. Exoskeleton and end-effector robots for upper and lower limbs rehabilitation: narrative review. PM&R. 2018;10:S174–88.

10. European Commission. Medical devices: guidance document - classification of medical devices [Internet]. United Kingdom Medicines and Healthcare products Regulation Agency; 2016 [cited 2018 Dec 10]. Available from: http://ec.europa.eu/growth/sectors/medical-devices/guidance/

11. Guiochet J, Hoang QAD, Kaaniche M, Powell DJ. Applying existing standards to a medical rehabilitation robot: Limits and challenges. IROS. 2012.

12. Hardwick RM, Caspers S, Eickhoff SB, Swinnen SP. Neural correlates of action: comparing meta-analyses of imagery, observation, and execution. Neuroscience and Biobehavioral Reviews. 2018;31–44.

13. Xu L, Zhang H, Hui M, Long Z, Jin Z, Liu Y, et al. Motor execution and motor imagery: a comparison of functional connectivity patterns based on graph theory. Neuroscience. 2014;261:184–94.

medRxiv preprint doi: https://doi.org/10.1101/2019.12.11.19014571; this version posted December 15, 2019. The copyright holder for this preprint (which was not certified by peer review) is the author/funder, who has granted medRxiv a license to display the preprint in perpetuity.
It is made available under a CC-BY-NC-ND 4.0 International license .

14. Sharma N, Baron JC. Does motor imagery share neural networks with executed movement: a multivariate fMRI analysis. Front Hum Neurosci. 2013;7:564–564.

15. Jeannerod M. Neural simulation of action: A unifying mechanism for motor cognition. NeuroImage. 2001;14:S103–9.

16. Mulder T. Motor imagery and action observation: cognitive tools for rehabilitation. J Neural Transm (Vienna). 2007;114:1265–78.

17. Vogt S, Di Rienzo F, Collet C, Collins A, Guillot A. Multiple roles of motor imagery during action observation. Frontiers in Human Neuroscience. 2013;7:807.

18. Friesen CL, Bardouille T, Neyedli HF, Boe SG. Combined Action Observation and Motor Imagery Neurofeedback for Modulation of Brain Activity. Frontiers in Human Neuroscience. 2017;10:692.

19. Eaves DL, Riach M, Holmes PS, Wright DJ. Motor imagery during action observation: A brief review of evidence, theory and future research opportunities. Frontiers in Neuroscience. 2016;10:514.

20. Kim T, Frank C, Schack T. A systematic investigation of the effect of action observation training and motor imagery training on the development of mental representation structure and skill performance. Frontiers in Human Neuroscience. 2017;11:499.

21. Li M, Xu G, Xie J, Chen C. A review: motor rehabilitation after stroke with control based on human intent. Proc Inst Mech Eng H. 2018;232:344–60.

22. Takahashi K, Domen K, Sakamoto T, Toshima M, Otaka Y, Seto M, et al. Efficacy of upper extremity robotic therapy in subacute poststroke hemiplegia: an exploratory randomized trial. Stroke. 2016;47:1385–8.

23. Fregni F, Pascual-Leone A. Hand motor recovery after stroke: tuning the orchestra to improve hand motor function. Cogn Behav Neurol. 2006;19:21–33.

24. Hallett M. Plasticity of the human motor cortex and recovery from stroke. Brain Res Brain Res Rev. 2001;36:169–74.

25. Zeiler SR, Krakauer JW. The interaction between training and plasticity in the poststroke brain. Curr Opin Neurol. 2013;26:609–16.

26. Mawase F, Uehara S, Bastian AJ, Celnik P. Motor learning enhances use-dependent plasticity. J Neurosci. 2017;37:2673–85.

27. Teplan M. Fundamentals of EEG measurement. Measurement Science Review. 2002;2.

28. Cohen MX. Analyzing Neural Time Series Data: Theory and Practice [Internet]. Cambridge; 2014. Available from: http://lib.ugent.be/catalog/rug01:002161004

29. Pfurtscheller G, Lopes da Silva FH. Event-related EEG/MEG synchronization and desynchronization: basic principles. Clin Neurophysiol. 1999;110:1842–57.

medRxiv preprint doi: https://doi.org/10.1101/2019.12.11.19014571; this version posted December 15, 2019. The copyright holder for this preprint (which was not certified by peer review) is the author/funder, who has granted medRxiv a license to display the preprint in perpetuity.
It is made available under a CC-BY-NC-ND 4.0 International license .

30. Laver KE, Lange B, George S, Deutsch JE, Saposnik G, Crotty M. Virtual reality for stroke rehabilitation. Cochrane Database Syst Rev. 2017;11:CD008349–CD008349.

31. Brookes J, Warburton M, Alghadier M, Mon-Williams M, Mushtaq F. Studying human behavior with virtual reality: The Unity Experiment Framework. Behavior Research Methods [Internet]. 2019; Available from: https://doi.org/10.3758/s13428-019-01242-0

32. Vourvopoulos A, Cardona JEM, Badia SB i. Optimizing motor imagery neurofeedback through the use of multimodal immersive virtual reality and motor priming. 2015 International Conference on Virtual Rehabilitation (ICVR). 2015. p. 228–34.

33. Johnston M, Bonetti D, Joice S, Pollard B, Morrison V, Francis JJ, et al. Recovery from disability after stroke as a target for a behavioural intervention: Results of a randomized controlled trial. Disability and Rehabilitation. 2007;29:1117–27.

34. Hülsmann F, Frank C, Senna I, Ernst MO, Schack T, Botsch M. Superimposed Skilled Performance in a Virtual Mirror Improves Motor Performance and Cognitive Representation of a Full Body Motor Action. Frontiers in Robotics and AI. 2019;6:43.

35. Monge-Pereira E, Ibanez-Pereda J, Alguacil-Diego IM, Serrano JI, Spottorno-Rubio MP, Molina-Rueda F. Use of electroencephalography brain-computer interface systems as a rehabilitative approach for upper limb function after a stroke: a systematic review. PM R. 2017;9:918–32.

36. Cervera MA, Soekadar SR, Ushiba J, Millan J d. R, Liu M, Birbaumer N, et al. Brain-computer interfaces for post-stroke motor rehabilitation: a meta-analysis. bioRxiv [Internet]. 2017; Available from: http://biorxiv.org/content/early/2017/11/24/224618.abstract

37. McConnell AC, Moioli RC, Brasil FL, Vallejo M, Corne DW, Vargas PA, et al. Robotic devices and brain-machine interfaces for hand rehabilitation post-stroke. Journal of Rehabilitation Medicine. 2017;49:449–60.

38. Fugl-Meyer AR, Jaasko L, Leyman I, Olsson S, Steglind S. The post-stroke hemiplegic patient. 1. a method for evaluation of physical performance. Scand J Rehabil Med. 1975;7:13–31.

39. Lyle RC. A performance test for assessment of upper limb function in physical rehabilitation treatment and research. International Journal of Rehabilitation Research [Internet]. 1981;4. Available from: https://journals.lww.com/intjrehabilres/Fulltext/1981/12000/A_performance_test_for_assessment_of_upper_limb.1.aspx

40. Matthews WB. Aids to the examination of the peripheral nervous system. Journal of the Neurological Sciences. 1977;33:299.

41. Office of the Director of Defense Research and Engineering Washington DC. Technology Readiness Assessment (TRA) Deskbook [Internet]. Fort Belvoir, VA, USA: Defense Technical Information Center; 2009 Jul. Report No.: ADA524200. Available from: https://apps.dtic.mil/dtic/tr/fulltext/u2/a524200.pdf

42. Maher CG, Sherrington C, Herbert RD, Moseley AM, Elkins M. Reliability of the PEDro scale for rating quality of randomized controlled trials. Physical Therapy. 2003;83:713–21.

medRxiv preprint doi: https://doi.org/10.1101/2019.12.11.19014571; this version posted December 15, 2019. The copyright holder for this preprint (which was not certified by peer review) is the author/funder, who has granted medRxiv a license to display the preprint in perpetuity.
It is made available under a CC-BY-NC-ND 4.0 International license .

43. PEDro Scale [Internet]. 1999 [cited 2018 Nov 30]. Available from: www.pedro.org.au/english/downloads/pedro-scale/

44. Belardinelli P, Laer L, Ortiz E, Braun C, Gharabaghi A. Plasticity of premotor cortico-muscular coherence in severely impaired stroke patients with hand paralysis. Neuroimage Clin. 2017;14:726–33.

45. Bergamasco M, Frisoli A, Fontana M, Loconsole C, Leonardis D, Troncossi M, et al. Preliminary results of BRAVO project: brain computer interfaces for Robotic enhanced Action in Visuo-motOr tasks. IEEE Int Conf Rehabil Robot. 2011;2011:5975377.

46. Broetz D, Braun C, Weber C, Soekadar SR, Caria A, Birbaumer N. Combination of brain-computer interface training and goal-directed physical therapy in chronic stroke: a case report. Neurorehabil Neural Repair. 2010;24:674–9.

47. Cincotti F, Pichiorri F, Arico P, Aloise F, Leotta F, de Vico Fallani F, et al. EEG-based brain-computer interface to support post-stroke motor rehabilitation of the upper limb. Conf Proc IEEE Eng Med Biol Soc. 2012;2012:4112–5.

48. George K, Iniguez A, Donze H, Kizhakkumthala S. Design, implementation and evaluation of a brain-computer interface controlled mechanical arm for rehabilitation. 2014 IEEE International Instrumentation and Measurement Technology Conference (I2MTC) Proceedings. 2014. p. 1326–8.

49. Ushiba J, Morishita A, Maeda T. A task-oriented brain-computer interface rehabilitation system for patients with stroke hemiplegia. 2014 4th International Conference on Wireless Communications, Vehicular Technology, Information Theory and Aerospace & Electronic Systems (VITAE). 2014. p. 1–3.

50. Rathee D, Chowdhury A, Meena YK, Dutta A, McDonough S, Prasad G. Brain–machine interface-driven post-stroke upper-limb functional recovery correlates with beta-band mediated cortical networks. IEEE Transactions on Neural Systems and Rehabilitation Engineering. 2019;27:1020–31.

51. Naros G, Gharabaghi A. Physiological and behavioral effects of beta-tACS on brain self-regulation in chronic stroke. Brain Stimul. 2017;10:251–9.

52. Norman S. Brain computer interface design for robot assisted neurorehabilitation [Internet]. University of California, Irvine; 2017. Available from: https://escholarship.org/uc/item/4v18v0d3

53. Pellegrino G, Tomasevic L, Tombini M, Assenza G, Bravi M, Sterzi S, et al. Inter-hemispheric coupling changes associate with motor improvements after robotic stroke rehabilitation. Restor Neurol Neurosci. 2012;30:497–510.

54. Bousseta R, El Ouakouak I, Gharbi M, Regragui F. EEG based brain computer interface for controlling a robot arm movement through thought. IRBM. 2018;39:129–35.

55. Formaggio E, Storti SF, Boscolo Galazzo I, Gandolfi M, Geroin C, Smania N, et al. Modulation of event-related desynchronization in robot-assisted hand performance: brain oscillatory changes in active, passive and imagined movements. J Neuroeng Rehabil. 2013;10:24.

medRxiv preprint doi: https://doi.org/10.1101/2019.12.11.19014571; this version posted December 15, 2019. The copyright holder for this preprint (which was not certified by peer review) is the author/funder, who has granted medRxiv a license to display the preprint in perpetuity.
It is made available under a CC-BY-NC-ND 4.0 International license .

56. Sarasola-Sanz A, Irastorza-Landa N, Lopez-Larraz E, Bibian C, Helmhold F, Broetz D, et al. A hybrid brain-machine interface based on EEG and EMG activity for the motor rehabilitation of stroke patients. IEEE Int Conf Rehabil Robot. 2017;2017:895–900.

57. Shiman F, Irastorza-Landa N, Sarasola-Sanz A, Spuler M, Birbaumer N, Ramos-Murguialday A. Towards decoding of functional movements from the same limb using EEG. Conf Proc IEEE Eng Med Biol Soc. 2015;2015:1922–5.

58. Muralidharan A, Chae J, Taylor DM. Extracting attempted hand movements from EEGs in people with complete hand paralysis following stroke. Front Neurosci. 2011;5:39.

59. Ono T, Mukaino M, Ushiba J. Functional recovery in upper limb function in stroke survivors by using brain-computer interface: a single case A-B-A-B design. Conf Proc IEEE Eng Med Biol Soc. 2013;2013:265–8.

60. Ang KK, Guan C, Phua KS, Wang C, Zhou L, Tang KY, et al. Brain-computer interface-based robotic end effector system for wrist and hand rehabilitation: results of a three-armed randomized controlled trial for chronic stroke. Frontiers in neuroengineering. 2014;7:30–30.

61. Barsotti M, Leonardis D, Loconsole C, Solazzi M, Sotgiu E, Procopio C, et al. A full upper limb robotic exoskeleton for reaching and grasping rehabilitation triggered by MI-BCI. 2015 IEEE International Conference on Rehabilitation Robotics (ICORR). 2015. p. 49–54.

62. Bundy DT, Souders L, Baranyai K, Leonard L, Schalk G, Coker R, et al. Contralesional brain-computer interface control of a powered exoskeleton for motor recovery in chronic stroke survivors. Stroke. 2017;48:1908–15.

63. Chowdhury A, Raza H, Meena YK, Dutta A, Prasad G. Online covariate shift detection based adaptive brain-computer interface to trigger hand exoskeleton feedback for neuro-rehabilitation. IEEE Transactions on Cognitive and Developmental Systems. 2018;1–1.

64. Chowdhury A, Meena YK, Raza H, Bhushan B, Uttam AK, Pandey N, et al. Active physical practice followed by mental practice using BCI-driven hand exoskeleton: a pilot trial for clinical effectiveness and usability. IEEE J Biomed Health Inform. 2018;22:1786–95.

65. Frolov AA, Mokienko O, Lyukmanov R, Biryukova E, Kotov S, Turbina L, et al. Post-stroke rehabilitation training with a motor-imagery-based brain-computer interface (BCI)-controlled hand exoskeleton: a randomized controlled multicenter trial. Frontiers in neuroscience. 2017;11:400–400.

66. Ono Y, Tominaga T, Murata T. Digital mirror box: an interactive hand-motor BMI rehabilitation tool for stroke patients. 2016 Asia-Pacific Signal and Information Processing Association Annual Summit and Conference (APSIPA). 2016. p. 1–7.

67. Norman SL, McFarland DJ, Miner A, Cramer SC, Wolbrecht ET, Wolpaw JR, et al. Controlling pre-movement sensorimotor rhythm can improve finger extension after stroke. Journal of Neural Engineering. 2018;15:056026.

68. Wang X, Wong W, Sun R, Chu WC, Tong KY. Differentiated effects of robot hand training with and without neural guidance on neuroplasticity patterns in chronic stroke. Frontiers in Neurology. 2018;9:810.

medRxiv preprint doi: https://doi.org/10.1101/2019.12.11.19014571; this version posted December 15, 2019. The copyright holder for this preprint (which was not certified by peer review) is the author/funder, who has granted medRxiv a license to display the preprint in perpetuity.
It is made available under a CC-BY-NC-ND 4.0 International license .

69. Tsuchimoto S, Shindo K, Hotta F, Hanakawa T, Liu M, Ushiba J. Sensorimotor connectivity after motor exercise with neurofeedback in post-stroke patients with hemiplegia. Neuroscience. 2019;416:109–25.

70. Carino-Escobar RI, Carillo-Mora P, Valdes-Cristerna R, Rodriguez-Barragan MA, Hernandez-Arenas C, Quinzaños-Fresnedo J, et al. Longtitudinal analysis of stroke patient' brain rhythms during an interview with a brain-computer interface. Neural Plasticity. 2019;2019:11.

71. Cantillo-Negrete J, Carino-Escobar RI, Elias-Vinas D, Gutierrez-Martinez J. Control signal for a mechatronic hand orthosis aimed for neurorehabilitation. 2015 Pan American Health Care Exchanges (PAHCE). 2015. p. 1–4.

72. Chowdhury A, Raza H, Dutta A, Nishad SS, Saxena A, Prasad G. A study on cortico-muscular coupling in finger motions for exoskeleton assisted neuro-rehabilitation. Conf Proc IEEE Eng Med Biol Soc. 2015;2015:4610–4.

73. Li M, He B, Liang Z, Zhao CG, Chen J, Zhuo Y, et al. An attention-controlled hand exoskeleton for the rehabilitation of finger extension and flexion using a rigid-soft combined mechanism. Frontiers in Neurorobotics. 2019;13:34.

74. Zhang J, Wang B, Zhang C, Xiao Y, Wang MY. An EEG/EMG/EOG-based multimodal human-machine interface to real-time control of a soft robot hand. Frontiers in Neurorobotics. 2019;13:7.

75. Randazzo L, Iturrate I, Perdikis S, Millán J d. R. mano: a wearable hand exoskeleton for activities of daily living and neurorehabilitation. IEEE Robotics and Automation Letters. 2018;3:500–7.

76. Tacchino G, Gandolla M, Coelli S, Barbieri R, Pedrocchi A, Bianchi AM. EEG analysis during active and assisted repetitive movements: evidence for differences in neural engagement. IEEE Trans Neural Syst Rehabil Eng. 2017;25:761–71.

77. Coffey AL, Leamy DJ, Ward TE. A novel BCI-controlled pneumatic glove system for home-based neurorehabilitation. Conf Proc IEEE Eng Med Biol Soc. 2014;2014:3622–5.

78. Holmes CD, Wronkiewicz M, Somers T, Liu J, Russell E, Kim D, et al. IpsiHand Bravo: an improved EEG-based brain-computer interface for hand motor control rehabilitation. Conf Proc IEEE Eng Med Biol Soc. 2012;2012:1749–52.

79. Stan A, Irimia DC, Botezatu NA, Lupu RG. Controlling a hand orthosis by means of P300-based brain computer interface. 2015 E-Health and Bioengineering Conference (EHB). 2015. p. 1–4.

80. Ramos-Murguialday A, Schürholz M, Caggiano V, Wildgruber M, Caria A, Hammer EM, et al. Proprioceptive feedback and brain computer interface (BCI) based neuroprostheses. PLOS ONE. 2012;7:e47048.

81. Ramos-Murguialday A, Birbaumer N. Brain oscillatory signatures of motor tasks. J Neurophysiol. 2015;113:3663–82.

medRxiv preprint doi: https://doi.org/10.1101/2019.12.11.19014571; this version posted December 15, 2019. The copyright holder for this preprint (which was not certified by peer review) is the author/funder, who has granted medRxiv a license to display the preprint in perpetuity.
It is made available under a CC-BY-NC-ND 4.0 International license .

82. Bauer R, Fels M, Vukelic M, Ziemann U, Gharabaghi A. Bridging the gap between motor imagery and motor execution with a brain-robot interface. Neuroimage. 2015;108:319–27.

83. Naros G, Naros I, Grimm F, Ziemann U, Gharabaghi A. Reinforcement learning of self-regulated sensorimotor beta-oscillations improves motor performance. Neuroimage. 2016;134:142–52.

84. Vukelic M, Gharabaghi A. Oscillatory entrainment of the motor cortical network during motor imagery is modulated by the feedback modality. Neuroimage. 2015;111:1–11.

85. Ono Y, Wada K, Kurata M, Seki N. Enhancement of motor-imagery ability via combined action observation and motor-imagery training with proprioceptive neurofeedback. Neuropsychologia. 2018;114:134–42.

86. Witkowski M, Cortese M, Cempini M, Mellinger J, Vitiello N, Soekadar S. Enhancing brain-machine interface (BMI) control of a hand exoskeleton using electrooculography (EOG). Journal of NeuroEngineering and Rehabilitation. 2014;11:165.

87. Fok S, Schwartz R, Wronkiewicz M, Holmes C, Zhang J, Somers T, et al. An EEG-based brain computer interface for rehabilitation and restoration of hand control following stroke using ipsilateral cortical physiology. Conf Proc IEEE Eng Med Biol Soc. 2011;2011:6277–80.

88. Diab MS, Hussain Z, Mahmoud S. Restoring function in paralyzed limbs using EEG. 2016 IEEE 59th International Midwest Symposium on Circuits and Systems (MWSCAS). 2016. p. 1–4.

89. King CE, Wang PT, Mizuta M, Reinkensmeyer DJ, Do AH, Moromugi S, et al. Noninvasive brain-computer interface driven hand orthosis. Conf Proc IEEE Eng Med Biol Soc. 2011;2011:5786–9.

90. Kam JWY, Griffin S, Shen A, Patel S, Hinrichs H, Heinze HJ, et al. Systematic comparison between a wireless EEG system with dry electrodes and a wired EEG system with wet electrodes. NeuroImage. 2019;184:119–29.

91. Mathewson KE, Harrison TJL, Kizuk SAD. High and dry? Comparing active dry EEG electrodes to active and passive wet electrodes. Psychophysiology. 2017;54:74–82.

92. Saab J, Battes B, Grosse-Wentrup M. Simultaneous EEG recordings with dry and wet electrodes in motor-imagery. In proceedings. Graz, Austria; 2011.

93. Lotte F, Guan C. Regularizing common spatial patterns to improve BCI designs: unified theory and new algorithms. IEEE Transactions on Biomedical Engineering. 2011;58:355–62.

94. Ang KK, Chin ZY, Wang C, Guan C, Zhang H. Filter bank common spatial pattern algorithm on BCI competition IV datasets 2a and 2b. Frontiers in neuroscience. 2012;6:39–39.

95. Bobrov PD, Korshakov AV, Roshchin VI, Frolov AA. Bayesian classifier for brain-computer interface based on mental representation of movements. Zh Vyssh Nerv Deiat Im I P Pavlova. 2012;62:89–99.

medRxiv preprint doi: https://doi.org/10.1101/2019.12.11.19014571; this version posted December 15, 2019. The copyright holder for this preprint (which was not certified by peer review) is the author/funder, who has granted medRxiv a license to display the preprint in perpetuity.
It is made available under a CC-BY-NC-ND 4.0 International license .

96. Oña ED, Cano-de la Cuerda R, Sanchez-Herrera P, Balaguer C, Jardon A. A review of robotics in neurorehabilitation: Towards an automated process for upper limb. J Healthc Eng. 2018;

97. Kersten P. Principles of physiotherapy assessment and outcome measures. Physical Management in Neurological Rehabilitation. 2004. p. 29–46.

98. Dovat L, Lambercy O, Ruffieux Y, Chapuis D, Gassert R, Bleuler H, et al. A haptic knob for rehabilitation after stroke. 2006 IEEE/RSJ International Conference on Intelligent Robots and Systems. Beijing, China: IEEE; 2006.

99. Abdalsalam E, Yusoff MZ, Kamel N, Malik AS, Mahmoud D. Classification of Four Class Motor Imagery for Brain Computer Interface. In: Ibrahim H, Iqbal S, Teoh SS, Mustaffa MT, editors. 9th International Conference on Robotic, Vision, Signal Processing and Power Applications. Springer Singapore; 2017. p. 297–305.

100. Grummett TS, Leibbrandt RE, Lewis TW, De Los Angeles D, Powers DMW, Willoughby JO, et al. Measurement of neural signals from inexpensive, wireless and dry EEG systems. Physiological Measurement. 2015;36.

101. Mladenov T, Kim K, Nooshabadi S. Accurate motor imagery based dry electrode brain-computer interface system for consumer applications. 2012 IEEE 16th International Symposium on Consumer Electronics. 2012. p. 1–4.

102. Guger C, Krausz G, Edliner G. Brain-computer interface control with dry EEG electrodes. Proceedings of the 5th International Brain-Computer Interface Conference. 2011. p. 316–9.

103. Srinivasan R. Methods to improve the spatial resolution of EEG. International Journal of Bioelectromagnetism. 1999;1:102–11.

104. Liao K, Xiao R, Gonzalez J, Ding L. Decoding individual finger movements from one hand using human EEG signals. PLOS ONE. 2014;9:e85192.

105. Johnson MJ, Micera S, Shibata T, Guglielmelli E. Rehabilitation and assistive robotics [TC Spotlight]. IEEE Robotics & Automation Magazine. 2008;15:16–110.

106. Arvaneh M, Guan C, Ang K, Quek C. Optimizing the Channel Selection and Classification Accuracy in EEG-Based BCI. Biomedical Engineering, IEEE Transactions on. 2011;58:1865–73.

1035

Table 2. Summary of Studies

Authors	Participants	Study Design	Task Design	BCI-Hand Robot	Main Outcomes
Studies involving stroke patients					
Ang et al., 2014 [60]	N=27 (7F:14M) Moderate to severe impairment of UE function Mean age: 54.2y Mean stroke duration: 385.1 days	3-armed RCT of motor function with MI-BCI-device as intervention Control groups: device only (Haptic Knob), SAT	Photo manipulation: hand opening and closing, pronation and supination Cue: visual (photo) Feedback: visual (photo) and kinaesthetic	EEG: 27 channels to classify ERD/ERS and coupled with EMG to confirm MI Device: Haptic Knob, 2-DOF for hand grasping and knob manipulation Actuation: DC brushed motors with linear belt drive Control: trigger	Clinical outcome measure: FMMA Distal, improvement in weeks 3, 6, 12, 24 BCI-device group = 2.5±2.4, 3.3±2.3, 3.2±2.7, 4.2±3.1 Device only group = 1.6±2.5, 2.9±3.0, 2.5±2.6, 2.5±3.0 SAT group = 0.4±1.1, 1.9±1.9, 1.0±1.3, 0.3±2.1
Barsotti et al., 2015 [61]	N=3 (1F:2M) Chronic stroke survivors with right arm hemiparesis Mean age: 62±12y	Probing MI classification by BCI training, time-frequency analysis and robot trajectories Uncontrolled	Reaching-grasping-releasing Cue: visual Feedback: kinaesthetic Minimum time required to perform MI = 2s	EEG: 13 channels to classify ERD Device: BRAVO 2-DOF hand orthosis attached to full UE exoskeleton Actuation: DC motors with rigid links Control: trigger	Mean classification accuracy during BCI training = 82.51±2.04% Average delay from visual cue to robot initiation = 3.45±1.6s Average delay due to patient's ability to start MI = 1.45s
Bundy et al., 2017 [62]	N=10 Chronic hemiparetic stroke with moderate to severe UE hemiparesis Mean age: 58.6±10.3y	Motor function evaluation before and after intervention by MI-BCI from unaffected hemisphere Uncontrolled	Opening of affected hand Cue: visual Feedback: visual and kinaesthetic	EEG: 8 channels to classify ERD Device: 3-pinch grip, 1-DOF hand exoskeleton	Clinical outcome measure: ARAT Score, improvement from baseline to completion (12 weeks) Mean ± SD = 6.20±3.81

Bundy et al. (cont'd)				Control: continuous depending on spectral power	Note: 5.7 ARAT Score is the minimal clinically important difference in chronic stroke survivors
Carino-Escobar et al. 2019 [70]	N=9 (4F:5M) Subacute ischaemic stroke Mean age: 59.9±2.8y Mean stroke duration: 158(±74)-185(±73) days	Determine longitudinal ERD/ERS patters and functional recovery with BCI-robot Uncontrolled	Extension-flexion of hand fingers Cue: visual (Graz MI) Feedback: visual and kinaesthetic	EEG: 11 channels to classify ERD/ERS Device: hand finger orthosis Actuation: DC motor with screw system for linear displacement, flexible links Control: trigger	FMA-UE: N=3 reported equal or higher than 3 score gains, N=3 no score gains, Mean longitudinal ERD/ERS: beta bands have higher association with time since stroke onset than alpha, and strong association with UL motor recovery
Chowdhury et al., 2018-b [63]	N=20 10 healthy and 10 hemiplegic stroke patients Mean age (healthy, stroke): 41±9.21y, 47.5±14.23y	Probe non-adaptive classifier (NAC) vs. Covariate Shift adaptive classifier (CSAC) of MI in EEG Control group: healthy participants	Extension-flexion of hand fingers Cue: visual Feedback: visual and kinaesthetic	EEG: 12 channels with EMG to classify ERD/ERS Device: EMOHEX 3-finger, 3-DOF each, exoskeleton (thumb, index, middle) Actuation: servomotors with rigid links Control: trigger	Mean classification accuracies during BCI training: Healthy group: calibration = 78.50±9.01%, NAC = 75.25±5.46%, CSAC = 81.50±4.89% Patient group: calibration = 79.63±13.11%, NAC = 70.25±3.43%, CSAC = 75.75±3.92%
Chowdhury et al., 2018-c [64]	N=4 (2F:2M) Hemiplegic stroke patients, right-handed, left hand impaired Mean age: 44.75±15.69y Mean stroke duration: 7 ±1.15mo	Motor function evaluation by using active physical practice followed by MI-BCI-controlled device intervention Uncontrolled	Extension-flexion of hand fingers Cue: visual Feedback: visual and kinaesthetic	EEG: 12 channels with force sensors to classify ERD/ERS Device: EMOHEX 3-finger, 3-DOF each, exoskeleton (thumb, index, middle) Actuation: servomotors with rigid links Control: trigger	Classification accuracies of 4 participants: P01 = 81.45±8.12%, P02 = 70.21±4.43%, P03 = 76.88±4.49%, P04 = 74.55±4.35% Clinical outcome measures: GS and ARAT Scores, improvement from baseline to completion (6 weeks) GS scores: group mean difference = +6.38 kg, p=0.06

Chowdhury et al., 2018-c (cont'd)					ARAT scores: group mean difference = +5.66, p<0.05
Frolov et al., 2017 [65]	N=74 (26F:48M) BCI 55: Control 19 Subacute or chronic stroke with mild to hemiplegic hand paresis, right-handed	Multi-centre RCT of MI-BCI-controlled hand exoskeleton Control group: SHAM	3 Tasks: (1) motor relaxation, (2) imagery of left-hand opening, (3) imagery of right-hand opening Cue: visual Feedback: visual and kinaesthetic	EEG: 30 channels to classify the three mental tasks by Bayesian classifier based on covariance matrices Device: hand exoskeleton by Neurobotics, Russia Actuation: pneumatic motors with spring flexors Control: trigger	Mean classification accuracy during BCI training = 40.6% Clinical outcome measures: FMMA Distal and ARAT Scores, improvement in 10 days of training FMMA Distal = 2.0, p<0.01 (BCI) and 1.0, p=0.046 (control) ARAT Grasp = 3.0, p<0.01 (BCI) and 1.0, p=0.0394 (control) ARAT Grip = 1.0, p<0.01 (BCI) and 1.0, p=0.045 (control) ARAT Pinch = 1.0, p<0.01 (BCI) and 0.0, p=0.675 (control)
Norman et al., 2018 [67]	N=8 (All male) Cortical and subcortical single haemorrhagic or ischaemic stroke (at least 6 months) Mean age: 59.5±11.8y	Implementation of sensorimotor rhythm (SMR) control on robot-assistive movement Uncontrolled	Extension of hand finger Cue: visual Feedback: visual and kinaesthetic	EEG: 16 channels mapping SMR changes Device: FINGER robot Actuation: Linear servo-tube actuator with rigid links Control: Visual - continuous (colour change respective to SMR), Robot - trigger	Mean classification accuracies: 8 participants: 83.1%, 76.3%, 73.3%, 68.2%, 74.5%, 86.5%, 47.9%, 40.0% Box and blocks test (BBT): At screening: mean score = 14.3±10.0, mean change after therapy = 4.3±4.5 (range 0-12). Higher score changes in participants who demonstrated SMR control but not significant (p=0.199)
Ono et al., 2016-a [66]	N=21 (9F:12M) Chronic stroke patients with hemiplegic hands Mean age: 57.9±2.4y	Probe congruent vs. incongruent MI feedback strategies Control groups: congruent (synchronous proprioceptive and visual feedback) and	Grasping of a tennis ball with a hand Cue: visual (video of hand performing action) Feedback: visual and kinaesthetic	EEG: 9 channels to classify ERD Device: Power Assist Hand - Team ATOM, Atsugi, Japan	Mean classification accuracies: Congruent feedback = 56.8±5.2%, chance level=36.4±4.5% Incongruent feedback = 40.0±3.5%, chance level 35.4±4.5%

Ono et al., 2016-a (cont'd)		incongruent (proprioceptive feedback given 1s after visual)		Actuation: pneumatic motors with rigid links Control: trigger	
Tsuchimoto et al., 2019 [69]	N=18 (3F:14M) Chronic haemorrhagic or ischaemic stroke (from 2mo onwards) Mean age: 58±10y	Implementation of MI-controlled robotic orthosis as neurofeedback Control: SHAM	Extension of hand finger Cue: unspecified Feedback: kinaesthetic and electrical stimulation	EEG: 5 channels to classify MI Device: robotic finger orthosis Actuation: servo motors with rigid links Control: trigger	Significant time-intervention interaction in the ipsilesional sensorimotor cortex. Higher coactivation of sensory and motor cortices for neurofeedback group in the ipsilesional sensorimotor cortices as compared to SHAM
Wang et al., 2018 [68]	N=24 (4F:20M) Chronic stroke patients with paralysed hands Mean age: 54±9y	Implementation of action observation and motor imagery (AO+MI) with kinaesthetic feedback Control: SHAM	Hand grasping Cue: visual (video of hand action / textual cues in SHAM group) Feedback: visual and kinaesthetic	EEG: 16 channels to classify ERD Device: robot hand Control: Trigger	AO+MI with kinaesthetic feedback group showed significant improvements in FMA-UE across longitudinal evaluation [$\chi2(2) = 7.659$, $p = 0.022$], no significant difference in SHAM group [$\chi2(2) = 4.537$, $p = 0.103$]
Authors	**Participants**	**Study Design**	**Task Design**	**BCI-Hand Robot**	**Main Outcomes**
Studies involving healthy participants					
Bauer et al., 2015 [71]	N=20 (11F:9M) Right-handed Mean age: 28.5±10.5y	Study on MI as compared to motor execution (ME) using BCI-device	Opening of left hand Cue: auditory Feedback: kinaesthetic	EEG: 31 channels to detect ERD, with EMG to classify MI from execution and account for tonic contraction Device: Amadeo, Tyromotion, Austria Control: discontinuation of ERD stops finger extension	Principal component analyses (between MI and execution) generated coefficients for the visual (VIS) and kinaesthetic (KIS) imagery scale, BCI-robot performance (BRI), tonic contraction task (MOC) and visuomotor integration task (VMI). VIS and KIS yielded high coefficients on MI while MOC and VMI yield high coefficients on ME. BRI show high coefficient yields on both MI and ME.

Cantillo-Negrete et al., 2015 [72]	N=1	Design and implementation of a MI-controlled hand orthosis	Extension-flexion of right-hand finger Cue: visual (modified Graz) Feedback: kinaesthetic	EEG: 11 channels to detect MI Device: 1-DOF hand finger orthosis Actuation: DC motor with screw system for linear displacement, flexible links Control: trigger	Correctly classified trials = 78%
Chowdhury et al., 2015-a [73]	N=6 Age range: 20-30y	Study of cortico-muscular coupling in robotic finger exoskeleton control	Extension-flexion of hand fingers Cue: visual Feedback: kinaesthetic	EEG: 10 channels with EMG to classify MI Device: 3-finger, 3-DOF each, exoskeleton (thumb, index, middle) Actuation: servomotors with rigid links Control: trigger	Mean classification accuracies: passive execution = 69.17%, hand execution = 71.25%, MI = 67.92%
Coffey et al., 2014 [74]	N=3 (All male) Right-handed Age range: 24-28y	Design and implementation of a MI-controlled hand orthosis	Hand digit and wrist contraction and extension Cue: visual (Graz MI) Feedback: kinaesthetic	EEG: 27 channels to classify MI Device: hand glove controlled by Arduino Actuation: pneumatic Control: trigger	Glove inflation-deflation cycle = 22s Classification accuracies of 3 participants: A = 92.5%, B = 90.0%, C = 80.0%
Diab et al., 2016 [75]	N=5	Design and implementation of EEG-triggered wrist orthosis with accuracy improvement	Hand opening and closing Cue: verbal instruction Feedback: kinaesthetic	EEG: 14 channels to detect hand movement-related EEG Device: actuated Talon wrist orthosis Actuation: linear Control: trigger	Mean classification accuracies: simulation studies = 95%, online BCI training = 86%

Fok et al., 2011 [76]	N=4	Design and implementation of a MI-controlled hand orthosis	Hand opening and closing Cue: unspecified Feedback: visual (cursor movement) and kinaesthetic	EEG: 14 channels to detect MI-related ERD Device: actuated Talon wrist orthosis Actuation: linear actuator Control: trigger	EEG signals from imagined hand movement was correlated with the contralesional hemisphere and utilised to trigger the actuation of orthosis ERD was detected from 12 Hz bin power of EEG during move condition
Li et al., 2019 [77]	N=14 (4F:10M) Mean age: 23.8±0.89y	Design and implementation of an attention-controlled hand exoskeleton with rigid-soft mechanism	Hand grasping Cue: visual (video of hand action) Feedback: kinaesthetic	EEG: 3 channels to map signals relative to attention Device: hand exoskeleton Actuation: linear actuator with rigid-soft mechanism Control: Trigger	Mean classification accuracy: 95.54% actuation success rate against the attention threshold
Holmes et al., 2012 [78]	N=6 (All male, young adults)	Design and implementation of a MI-controlled hand orthosis	Hand opening and closing Cue: textual Feedback: kinaesthetic	EEG: 14 channels to detect hand movement-related EEG Device: ExoFlex Hand Exoskeleton controlled by Arduino Actuation: linear actuator connected to chained links that flex Control: trigger	Classification accuracies of 6 participants: T001 = 95%, T002 = 98%, D001 = 91%, U001 = 93%, E001 = 87%, E002 = 86%
King et al., 2011 [79]	N=1 (Female) 24y	Contralateral control of hand orthosis using EEG-based BCI	Right hand idling and grasping Cue: textual Feedback: visual and kinaesthetic	EEG: 63 channels to control contralateral hand movement Device: hand orthosis	Offline classification accuracy = 95.3±0.6%, $p < 3.0866\times10^{-25}$ Average lag from voluntary contractions to BCI-robot control = 2.24 ± 0.19s (after 5 sessions)

King et al. (cont'd)				Actuation: servomotors attached to Bowden cables as tendons Control: trigger	
Naros et al., 2016 [80]	N=32 (16F:16M) Mean age: 25.9±0.5y	2x2 factorial design with parameters: adaptive classifier threshold and non-adaptive classifier threshold, contingent feedback and non-contingent feedback	Opening of right hand Cue: auditory Feedback: kinaesthetic	EEG: 32 channels to detect ERD, with EMG to classify MI (FC3, C3, CP3 used) Device: Amadeo, Tyromotion, Austria Control: trigger	Significant enhancement in group 1 (adaptive classifier + contingent feedback), p=0.0078 Significant reduction in group 4 (non-adaptive classifier + non-contingent feedback), p=0.0391 Motor performance improvement over baseline from first and last tasks, significant results: Group 1 (adaptive classifier + contingent feedback), p=0.0313 Group 4 = (non-adaptive classifier + non-contingent feedback), p=0.0411
Ono et al., 2018-b [81]	N=28 Right-handed except 1	Implementation of an action observation strategy with visual and proprioceptive, or auditory feedback to MI Control group: SHAM	Grasping of a tennis ball with a hand Cue: visual (video of hand performing action) Feedback: visual, kinaesthetic and auditory	EEG: 9 channels to classify ERD Device: Power Assist Hand - Team ATOM, Atsugi, Japan Actuation: pneumatic motors with rigid links Control: trigger	AO+MI + proprioceptive and visual feedback: Mean MI-ERD powers of correct feedback vs SHAM provide significant interaction, $F_{1,17}$=6.618, p=0.020 (6 days) Statistically significant increase in MI-ERD power in correct feedback group over baseline, p=0.012 (6 days)
Stan et al., 2015 [82]	N=9	Trigger a hand orthosis using a P300 speller BCI	Spell E (enable), A (hand opening) and B (hand closing) in P300 speller BCI to perform hang grasping, moving and releasing objects Cue: textual (spelling)	EEG: 8 channels focusing on visual cortex Device: hand orthosis Actuation: 2 servomotors and	Mean classification accuracies: 100% (on 6th letter flash during calibration)

Stan et al. (cont'd)			Feedback: visual (textual) and kinaesthetic	current feedback circuitry Control: trigger	
Ramos-Murguialday et al., 2012 [83]	N=23 Mean age (contingent positive, contingent negative, SHAM): 26.6±4y, 26.5±5y, 26.2±2y	Probing MI with proprioceptive feedback Experimental groups: contingent positive, contingent negative feedback Control group: SHAM	5 tasks: MI without direct control, MI with direct control, passive, active, rest Cue: auditory Feedback: visual and kinaesthetic	EEG: 61 channels with EMG to classify ERD/ERS Device: hand orthosis Actuation: DC motor M-28 with a worm gearhead and Bowden cables for each finger Control: trigger	Contingent positive feedback provided higher BCI performance during MI without feedback than contingent negative and SHAM; and higher during MI with or without feedback as compared to rest
Ramos-Murguialday and Birbaumer, 2015 [84]	N=9 Right-handed Mean age: 26.6±4y	Detect oscillatory signatures of motor tasks during EEG	5 tasks: MI without direct control, MI with direct control, passive, active, rest Cue: auditory Feedback: visual and kinaesthetic	EEG: 61 channels with EMG to classify ERD/ERS Device: hand orthosis Actuation: DC motor M-28 with a worm gearhead and Bowden cables for each finger Control: trigger	Significant change in power in all frequency ranges during MI with direct control before trial initiation Kinaesthetic feedback increased significant changes in alpha and beta power; therefore, increasing BCI performance
Randazzo et al., 2018 [85]	N=9 (2F:7M) Mean age: 23±5y	Design and implementation of a hand orthosis with testing of kinaesthetic effects in EEG	4 tasks: rest (REST), exoskeleton-induced hand motions (EXO), MI of right hand (MI), exoskeleton-induced hand motions plus MI (MIEXO) Cue: visual Feedback: kinaesthetic	EEG: 16 channels to detect MI Device: mano hand exoskeleton Actuation: linear servomotors attached to Bowden cables as tendons Control: passive (exoskeleton not dependent on MI to	Mean classification accuracies among groups: (vs REST) MI = 63.02±5.91%, EXO = 69.64±5.74%, MIEXO = 72.19±6.57% MIEXO vs EXO = 69.91±9.86% Chance level at 95% confidence = 58% (N=50 trials)

Randazzo et al. (cont'd)				move during MIEXO task)	
Tacchino et al., 2017 [86]	N=8 (7F:1M) Right-handed Mean age: 26.3±1.9y	2x2 factorial design with parameters: glove, no glove, active movement, passive movement	Opening and closing of hand, 4 tasks: (A) glove with active movement, (B) glove with passive movement, (C) no glove with active movement, (D) no glove and no movement Cue: auditory Feedback: kinaesthetic	EEG: 19 channels with EMG to detect ERD/ERS (C3, F3, Cz used) Device: Gloreha hand rehabilitation glove Actuation: electric actuators with Bowden cables on each finger Control: passive (glove not dependent on brain-state during tasks)	Statistically significant ERD changes in beta and mu bands were observed to initiate earlier in tasks A and C (involves active movement) Stronger and longer ERD was observed in tasks A and B (involves robotic assistance) suggesting reinforced afferent kinaesthetic feedback
Vukelic and Gharabaghi, 2015 [87]	N=11 (4F:7M) Right-handed Mean age: 25.83±3.1y	Assessment sensorimotor activity during MI with either visual or kinaesthetic feedback	Right hand opening Cue: visual (coloured cursor ball) Feedback: visual and kinaesthetic (separated by experimental groups)	EEG: 128 channels to detect ERD/ERS during MI (F3, CP3, C3 used) Device: Amadeo, Tyromotion, Austria Control: trigger	MI + kinaesthetic feedback group resulted in higher beta ERS (p=0.02) during rest and higher beta ERD (p=0.04) during MI Kinaesthetic feedback provides higher stability and sustained beta ERD activity than visual feedback
Witkowski et al., 2014 [88]	N=12 (4F:8M) Right-handed Mean age: 28.1±3.63y	Assessment performance and safety of EEG-EOG hybrid BCI	Right hand grasping Cue: visual (coloured squares and arrows) Feedback: kinaesthetic	EEG: 5 channels with EOG and EMG to detect ERD during MI Device: HX hand exoskeleton Actuation: DC motors with Bowden cables for thumb and index fingers Control: trigger	Mean classification accuracies: EEG only = 63.59±10.81% EEG/EOG hybrid = 60.77±9.42% Mean safety criterion violations during rest: EEG only = 45.91±26.8% EEG/EOG hybrid = 10.14±0.3%

Zhang et al., 2019 [89]	N=6 (2F:4M) Right-handed Age range: 23-26y	Implementation of a multimodal system using EEG, EMG and EOG to control a soft-robotic hand	Graz visualisation and auditory instructions, eye movements and physical practice (hand gestures) Cue: visual (Graz MI), auditory Feedback: visual and kinaesthetic	EEG with EMG and EOG: 40 channels to analyse ERD/ERS patterns Device: Soft pneumatic finger Actuation: pneumatic actuator with soft structures Control: trigger	Mean classification accuracies: EOG = 94.23% EEG = 31.46% EMG = 36.38% Multimodal = 93.83±0.02%

UE = Upper Extremity, MI = Motor Imagery, BCI = Brain-Computer Interface, RCT = Randomised Clinical Trial, SAT = Standard Arm Therapy, EMG = Electromyography, EOG = Electrooculography, ERD/ERS = Event-Related Desynchronisation/Synchronisation, FMMA = Fugl-Meyer Motor Assessment, ARAT = Action Research Arm Test, GS = Grip Strength, DOF = Degrees-of-Freedom