

1           **Heat inactivating and reusing of virus-contaminated disposable**

2   **medical mask**

3      Running title: Inactivating virus-contaminated medical mask for reuse

4      Wuhui Song<sup>1#</sup>, Bin Pan<sup>2#</sup>, Haidong Kan<sup>2</sup>, Yanyi Xu<sup>2\*</sup>, Zhigang Yi<sup>1,3\*</sup>

5  
6      1.Key Laboratory of Medical Molecular Virology (MOE/NHC/CAMS), School of  
7      Basic Medical Sciences, Fudan University , Shanghai 200032, China

8  
9      2.Department of Environmental Health, School of Public Health, Fudan University,  
10     Shanghai 200032, China

11  
12     3. Shanghai Public Health Clinical Center, Fudan University, Shanghai 200032, China

13  
14     # Co-first authors

15  
16     \* Corresponding authors: [yanyi\\_xu@fudan.edu.cn](mailto:yanyi_xu@fudan.edu.cn); [zgyi@fudan.edu.cn](mailto:zgyi@fudan.edu.cn)

17     138 YiXueYuan Road, Shanghai 200032, People's Republic of China

18  
19  
20     **Key words:** Heat inactivation; Medical mask; Filterability; Influenza virus; 2019

21     novel coronavirus

22  
23     **NOTE:** This preprint reports new research that has not been certified by peer review and should not be used to guide clinical practice.

24 **Abstract:**

25 As the prevalence of COVID-19 in all the area of China and continuous spread to  
26 many other countries, it is in urgent need of medical mask for community people. We  
27 have reported a simple method to inactivate artificially influenza virus-contaminated  
28 medical mask without affecting the filterability of mask by heating with hair dryer for  
29 30min. In this study, we extended our studies to optimize our protocols and evaluate  
30 the filterability of mask after several-rounds of heat treatment. We found that baking  
31 at 70°C for 30min almost completely inactivated virus as hair dryer treatment for  
32 30min described before. One-round of heat treatment with hair dryer for 30min or  
33 baking at 70°C for 30min did not affect filterability of mask whilst two-rounds of  
34 treatment slightly but significantly reduced filterability of mask. Thus, heating with  
35 hair dryer for 30min or baking at 70°C for 30min can inactive contaminated medical  
36 mask and the treated mask can be reused at least once.

37

38

## 39 **Introduction:**

40 Since the outbreak of COVID-19 in Wuhan China, it was endemic to all over the  
41 China within less than one month, causing over 80000 cases and over 3000 mortalities  
42 in China. It is considered to have pandemic potential, as it has been spread to almost  
43 all the continents and has caused over 20000 cases outside China. COVID-19 is  
44 caused by infection with a novel coronavirus SARS-CoV-2<sup>1-3</sup>, and its  
45 human-to-human transmission occurs mainly through close contacts<sup>4</sup>. Personal  
46 protective equipment (PPE) like medical mask is critical for public to prevent the  
47 infection of COVID-19. Thus it is in urgent need of medical mask all over the world.  
48 However, there is global shortage of medical mask. Medical mask acts similarly as  
49 N95 respirators for preventing Influenza virus infection<sup>5</sup>. Re-use of disposable  
50 medical mask would alleviate the panic of shortage of mask. Prior to re-use of mask,  
51 we should inactivate potential contaminated virus on the mask. Heat inactivation of virus  
52 such as incubating at 56°C for 30min is widely accepted to be able to inactivate  
53 enveloped virus like influenza virus and coronavirus. And importantly, heating at  
54 70 °C for 24 hour does not significantly change the filtration efficiency of  
55 polypropylene (PP)<sup>6</sup>, a core matrix for medical mask, whereas conventional  
56 disinfectant like ethanol dramatically destroys filter performance of polypropylene  
57 electret filters<sup>7</sup>. We have developed a simple method to inactivate medical mask that  
58 is artificially contaminated by influenza virus via heating with hair dryer for 30min  
59 without affecting its filterability<sup>8</sup>, which can be easily adapted by public. In this study,

60 we extended our studies to optimize our protocols by shortening treatment intervals  
61 with hair dryer and baking mask at different temperatures. We demonstrated that hair  
62 dryer treatment for 15 min did not effectively inactivate influenza virus (IVA) on  
63 medical mask compared with 30 min as described before. And that baking at 70°C for  
64 30 min effectively inactivated IVA on mask whereas baking at 65°C for 30 min did  
65 not. We also evaluated the filterability of mask after several-rounds of heat treatment.  
66 Our results reveal that two-rounds of treatment with hair dryer for 30min or baking at  
67 70°C for 30min significantly reduced filterability of mask but one-round of treatment  
68 did not affect filterability of mask. Thus, we provided a simple method for reuse of  
69 disposable medical mask, which may help tackle the urgent need of medical mask  
70 during COVID-19 prevalence.

71

## 72 **Materials and Methods**

### 73 **Cell and virus**

74 Madin-Darby canine kidney (MDCK) cells were purchased from Cell Bank of  
75 the Chinese Academy of Sciences, Shanghai, China ([www.cellbank.org.cn](http://www.cellbank.org.cn)) and  
76 maintained in Dulbecco's modified medium supplemented with 10% FBS (Gibco) and  
77 25mM HEPES (Gibco) with non-essential amino acids (Gibco). Influenza A(H1N1)  
78 A/PR8 were purchase from ATCC and propagated in MDCK cells.

### 79 **Heat treatment of medical mask**

80 Medical mask was mock-contaminated by dropping a 10 $\mu$ l of IVA solution  
81 containing  $3.6 \times 10^5$  pfu of IVA in 3 different sites on medical mask where each site  
82 was marked with a square. Due to the hydrophobic property of mask, liquid drop is  
83 difficult be absorbed onto the surface of the mask. The virus drop was doted on  
84 between the kink marks of the mask. Then the mask was wrapped with a food storage  
85 bag and then heat treated with hair dryer (1400w, 50Hz) by moving around over the  
86 surface of the wrapped mask vertically at a distance of about 10~20cm. Alternatively,  
87 the wrapped mask was moved into baking oven and treated at indicated temperatures  
88 with various intervals.

### 89 **Rescue of the virus from mask**

90 After heat treatment, the traces of IVA drop were visible within the marked  
91 squares. Due to the hydrophobic property of mask, the virus within the marked  
92 squares could be easily rescued by pipetting 250 $\mu$ l of Viral Transport Media (Hank's  
93 Balanced Salt Solution (1X HBSS) supplemented with 0.1% bovine serum albumin  
94 (BSA), 100 units/ml penicillin G and 100 units/ml streptomycin)<sup>9</sup> onto the traces until

95 the traces disappear, then 125 $\mu$ l of the rescued virus was used for infecting naïve  
96 MDCK cells in the presence of 5 $\mu$ g/ml TPCK-trypsin (sigma) for 1 hour at 37°C in a  
97 cell culture incubator. After wash with DMEM media for 4 times, fresh DMEM media  
98 with 1 $\mu$ g/ml TPCK-trypsin was added. At indicated time points post infection, the  
99 supernatants were collected.

#### 100 **Viral RNA quantification**

101 The RNAs in the supernatants from the infected MDCK cells were extracted by  
102 QIAamp Viral RNA kit (Qiagen) according to the manufacturers' protocol. RNAs  
103 were eluted in H<sub>2</sub>O and quantified by a Taqman-based real time PCR with One Step  
104 PrimeScript RT-PCR kit (Takara) according to the manufacturers' protocol with  
105 400nM of each primer (sense primer: CTT CTA ACC GAG GTC GAA ACG TA,  
106 anti-sense primer: GGT GAC AGG ATT GGT CTT GTC TTT A) and 200nM of  
107 probe (FAM-TCA GGC CCC CTC AAA GCC GAG-BHQ1). The relative RNA  
108 levels were calculated by 2<sup>- $\Delta$ CT</sup> method <sup>10</sup>.

#### 109 **PM<sub>2.5</sub> filterability measurement**

110 A suction flask (Shuniu, 250mL, GG-17) together with the particulate matter  
111 monitor (TSI, AM510) were used to evaluate the PM<sub>2.5</sub> filterability of medical masks  
112 (YINUO, FE3) before and after heat treatment. Considering the effect of suction  
113 process on the filtration performance of the masks, 5 experimental groups were set up  
114 as following:1). Untreated group (clean unused masks without any treatment); 2).  
115 One-round use + baking group (masks are used under normal condition for 4 hours  
116 and then baked in oven at 70°C for 30min); 3). Two-round use+ baking group (masks

117 are used under normal condition for 8 hours, with incubation in oven at 70°C for  
118 30min every 4 hours); 4). One-round use + hair dryer group (masks are used under  
119 normal condition for 4 hours and then heat treated by hair dryer for 30min as  
120 described above); 5). Two-round use + hair dryer group (masks are used under normal  
121 condition for 8 hours, with heat treatment by air dryer for 30min every 4 hours).  
122 Masks ( $N=3$ /group) were tightly bound to the top of the suction flask, while the  
123 particulate matter monitor was used to detect the  $PM_{2.5}$  concentrations near the top  
124 and the side outlet of the flask. The total suction filtration process lasted for 4 hours,  
125 and the tested flow rate is 1.8 L/min.  $PM_{2.5}$  concentrations were recorded every 30min,  
126 and repeated for 3 times at each time point.

127

## 128 **Results**

### 129 **Heat inactivation of IVA on mock-contaminated medical mask**

130 In our previous study, baking at 56°C for 30 min only partially inactivated IVA  
131 on medical mask, with a 1~3 log reduction of viral RNA level, comparing to 6 log  
132 reduction of viral RNA level after hair dryer treatment for 30 min<sup>8</sup>. In the present  
133 study, we first increased baking temperature and treated IVA mock-contaminated  
134 medical mask at 65°C for 30 min. After treatment, the virus on the mask was rescued  
135 and used to re-infect MDCK cells. Then we collected the supernatants of the infected  
136 cells at 0 and 48 hours post infection and quantified the viral RNA levels by real-time  
137 PCR. The inactivation efficiency was assessed by reduction of the viral RNA level  
138 comparing to the un-treated group. Baking at 65°C for 30 min resulted in 2~5 log  
139 reduction of viral RNA level but did not reduce viral RNA level to basal level (level  
140 at 0 hour post infection) (Fig 1A). Hair dryer treatment for 30 min nearly completely  
141 inactive IVA on medical mask<sup>8</sup>, while for convenience, we sought to shorten the  
142 treatment intervals. We assessed the inactivation efficiency of hair dryer treatment for  
143 5, 10 and 15 min as described above. As shown in Figure 1A, hair dryer treatment for  
144 5, 10 and 15 min did not effectively inactive IVA.

145 Then we continued to optimize baking conditions and increase temperature to  
146 70°C. We treated IVA-contaminated medical mask at 70°C for 15 min and 30 min and  
147 assessed the viral replication level of the rescued virus. As shown in Figure 1B,  
148 baking at 70°C for 15 min and 30 min both effectively reduced viral RNA levels to  
149 nearly basal levels and treatment for 30 min was more effective than treatment for  
150 15min. Thus heat treatment with hair dryer for 30min<sup>8</sup> and baking at 70°C for 30 min  
151 both effectively inactive IVA-contaminated medical mask.



## 152 **PM<sub>2.5</sub> filterability of medical masks after heat treatment**

153 We assessed protective function of medical mask by measuring the filterability  
154 of medical masks to ambient PM<sub>2.5</sub> after similar heat treatment as described before <sup>8</sup> .  
155 To evaluate the recycle times of the medical mask, masks were subjected to several  
156 rounds of wear (use) and heat treatment. Masks were used under normal condition for  
157 4 hours followed by treatment with hair dryer for 30min or baking at 70°C for 30 min,  
158 and then subjected to a 4-hour suction process mimicking the usage scenario by an  
159 adult under normal condition. As demonstrated in Figure 2A, PM<sub>2.5</sub> filtration rate of  
160 all the tested disposable medical masks was slightly changed during the 4-hour  
161 suction process. In general, the filterability remained stable with PM<sub>2.5</sub> filtration rate  
162 above 85% at all the tested time points. Among all the experimental groups, masks  
163 that have been used and heat treated once (by baking or hair dryer) have similar  
164 4-hour average PM<sub>2.5</sub> filtration rate compared to the untreated ones (Figure 2B).  
165 However, after being used and heat-treated twice (by baking or hair dryer), their  
166 filtration efficiency was significantly reduced as shown in Figure 2B. Our results  
167 indicate that heat inactivation by baking or hair dryer for 30 min may serve as an  
168 effective way for reuse of disposable medical masks, but this method is not  
169 encouraged to be used for more than once.

170

## 171 **Discussion**

172 It is not suggested to reuse disposable medical mask, especially for people who  
173 are in close contact with patients, medical staffs and laboratory technicians. But for  
174 community people who are at relative low risk of contacting high dosage of  
175 SARS-CoV-2, it is plausible to reuse medical mask after reliable inactivating  
176 treatment during the COVID-19 prevalence, which may alleviate the heavily global  
177 shortage of medical mask. We used IVA to mimic SARS-CoV-2 as they transmit  
178 similarly and both have envelopes and mock contaminated medical mask by dotting  
179 IVA drops onto the mask, then inactivated the IVA on medical mask by convenient  
180 heat treatment with hair dryer and baking that are easily to be adapted by community  
181 people. We found that baking at 70°C for 30min almost completely inactivated virus  
182 as hair dryer treatment for 30min described before <sup>8</sup>. But baking at 56°C and 65°C  
183 for 30min could not effectively activate virus <sup>8</sup>(Fig. 1A). Incubating at 56°C for  
184 30min is a widely used protocol to inactivate influenza virus or coronavirus in  
185 solution. The incomplete inactivation by baking at this temperature and at 65°C  
186 indicates that baking a surface has less efficiency than incubating in solution.  
187 Maintaining the filter function of medical mask during usage is critical for preventing  
188 virus infection. We demonstrated that one-round of heat treatment did not affect  
189 filterability of mask whilst two-rounds of treatment slightly but significantly reduced  
190 filterability of mask. Thus, we provided a simple method for reuse of medical mask  
191 by heating with hair dryer for 30min or baking at 70°C for 30min and the treated  
192 mask can be reused at least once.

193 **Acknowledgements**

194 This work was inspired by professor Yuemei Wen. We are grateful to Chun-fai  
195 Yung and many other colleagues for their kind suggestions and inputs. This work was  
196 supported in part by the National Science and Technology Major Project of China  
197 (2017ZX10103009). Key Emergency Project of Shanghai Science and Technology  
198 Committee (20411950103). The funders had no role in study design, data collection  
199 and analysis, decision to publish, or preparation of the manuscript.

200 **Conflict of Interest**

201 The authors declare no conflict of interest.

202

203 **Reference:**

- 204 1. Zhu N, Zhang D, Wang W, et al. A Novel Coronavirus from Patients with  
205 Pneumonia in China, 2019. *The New England journal of medicine*.  
206 2020;382(8):727-733.
- 207 2. Zhou P, Yang XL, Wang XG, et al. A pneumonia outbreak associated with a  
208 new coronavirus of probable bat origin. *Nature*. 2020.
- 209 3. Chen L, Liu W, Zhang Q, et al. RNA based mNGS approach identifies a novel  
210 human coronavirus from two individual pneumonia cases in 2019 Wuhan  
211 outbreak. *Emerging microbes & infections*. 2020;9(1):313-319.
- 212 4. Li Q, Guan X, Wu P, et al. Early Transmission Dynamics in Wuhan, China, of  
213 Novel Coronavirus-Infected Pneumonia. *The New England journal of*  
214 *medicine*. 2020.
- 215 5. Radonovich LJ, Jr., Simberkoff MS, Bessesen MT, et al. N95 Respirators vs  
216 Medical Masks for Preventing Influenza Among Health Care Personnel: A  
217 Randomized Clinical Trial. *Jama*. 2019;322(9):824-833.
- 218 6. Zhang H, Liu J, Zhang X, Huang C, Jin X. Design of electret polypropylene  
219 melt blown air filtration material containing nucleating agent for effective  
220 PM2.5 capture. *RSC Adv*. 2018;8:7932-7941.
- 221 7. Choi H, Park E, Kim J, Kim S, Lee M. Experimental Study on Charge Decay  
222 of Electret Filter Due to Organic Solvent Exposure. *Aerosol Science and*  
223 *Technology*. 2015;49:977-983.
- 224 8. Song W, Pan B, Kan H, Xu Y, Yi Z. Evaluation of heat inactivation of virus

- 225           contamination on medical mask. *Journal of Microbes and Infection*.  
226           2020;15(1):31-35.
- 227    9.       Blachere FM, Lindsley WG, McMillen CM, et al. Assessment of influenza  
228           virus exposure and recovery from contaminated surgical masks and N95  
229           respirators. *Journal of virological methods*. 2018;260:98-106.
- 230    10.      Livak KJ, Schmittgen TD. Analysis of relative gene expression data using  
231           real-time quantitative PCR and the 2(-Delta Delta C(T)) Method. *Methods*.  
232           2001;25(4):402-408.
- 233
- 234

235 **Figure Legends**

236 **Figure 1. Assessment of efficiency of heat inactivation of IVA on mask.** After  
237 indicated heat treatment, IVA on the mask was rescued and used to infect naïve  
238 MDCK cells. After extensive wash, the supernatants were collected at 0 and 48 hours  
239 post infection (H.P.I) and the virus in the supernatants were quantified by q-PCR. The  
240 RNA copy levels relative to that of the untreated (48 h) group were calculated and  
241 plotted. Mean  $\pm$  SEM are shown (n=3).


242 **Figure 2. M<sub>2.5</sub> filterability of disposable medical masks.** After one-round or  
243 two-round use and heat treatment, the filtration rate was measured. A. PM<sub>2.5</sub> filtration  
244 rate change during the 4-hour suction process. \* $p$ <0.05 versus untreated group at the  
245 same time point, One-way ANOVA; B. Average PM<sub>2.5</sub> filtration rate within the  
246 suction process were plotted. \* $p$ <0.05 versus untreated group, One-way ANOVA.  
247 Mean  $\pm$  SD are shown (n=3).

248

249

250 **Figure 1**

251

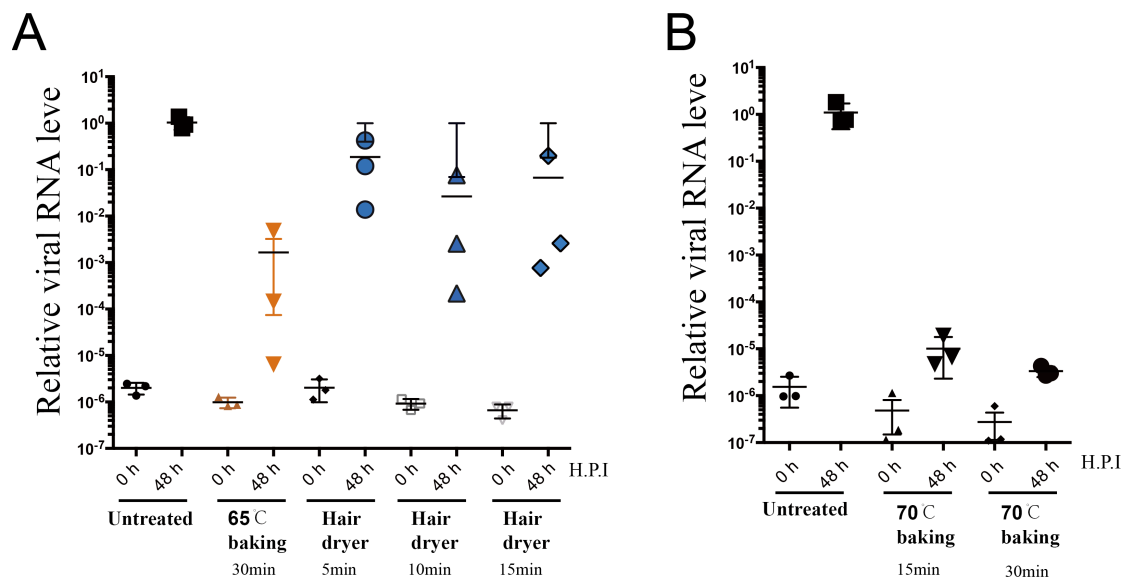

252

253 **Figure 1. Assessment of efficiency of heat inactivation of IVA on mask. After**

254 indicated heat treatment, IVA on the mask was rescued and used to infect naïve

255 MDCK cells. After extensive wash, the supernatants were collected at 0 and 48 hours

256 post infection (H.P.I) and the virus in the supernatants were quantified by q-PCR. The


257 RNA copy levels relative to that of the untreated (48 h) group were calculated and

258 plotted. Mean  $\pm$  SEM are shown (n=3).

259

260 **Figure 2**

261

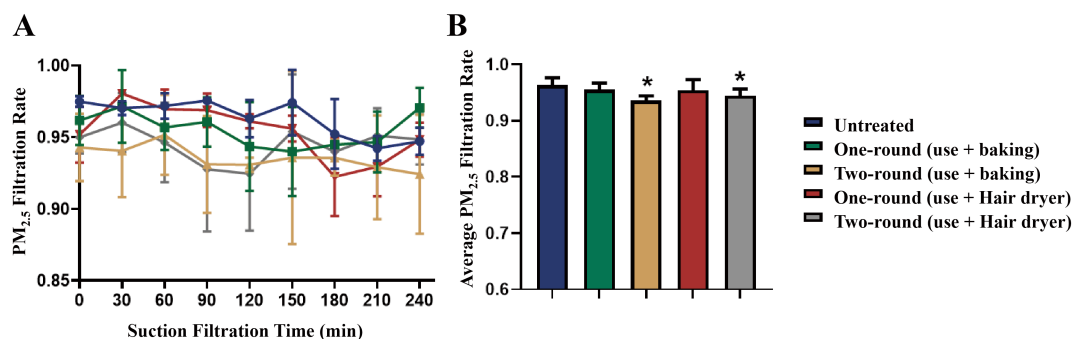

262

263 **Figure 2. PM<sub>2.5</sub> filterability of disposable medical masks.** After one-round or

264 two-round use and heat treatment, the filtration rate was measured. A. PM<sub>2.5</sub> filtration

265 rate change during the 4-hour suction process. \**p* < 0.05 versus untreated group at the

266 same time point, One-way ANOVA; B. Average PM<sub>2.5</sub> filtration rate within the

267 suction process were plotted. \**p* < 0.05 versus untreated group, One-way ANOVA.

268 Mean ± SD are shown (n=3).

269

270

271

272