

24 **Abstract:**

25 As the prevalence of COVID-19 in all the area of China and continuous spread to
26 many other countries, it is in urgent need of medical mask for community people. We
27 have reported a simple method to inactivate artificially influenza virus-contaminated
28 medical mask without affecting the filterability of mask by heating with hair dryer for
29 30min. In this study, we extended our studies to optimize our protocols and evaluate
30 the filterability of mask after several-rounds of heat treatment. We found that baking
31 at 70°C for 30min almost completely inactivated virus as hair dryer treatment for
32 30min described before. One-round of heat treatment with hair dryer for 30min or
33 baking at 70°C for 30min did not affect filterability of mask whilst two-rounds of
34 treatment slightly but significantly reduced filterability of mask. Thus, heating with
35 hair dryer for 30min or baking at 70°C for 30min can inactive contaminated medical
36 mask and the treated mask can be reused at least once.

37

38

39 **Introduction:**

40 Since the outbreak of COVID-19 in Wuhan China, it was endemic to all over the
41 China within less than one month, causing over 80000 cases and over 3000 mortalities
42 in China. It is considered to have pandemic potential, as it has been spread to almost
43 all the continents and has caused over 20000 cases outside China. COVID-19 is
44 caused by infection with a novel coronavirus SARS-CoV-2¹⁻³, and its
45 human-to-human transmission occurs mainly through close contacts⁴. Personal
46 protective equipment (PPE) like medical mask is critical for public to prevent the
47 infection of COVID-19. Thus it is in urgent need of medical mask all over the world.
48 However, there is global shortage of medical mask. Medical mask acts similarly as
49 N95 respirators for preventing Influenza virus infection⁵. Re-use of disposable
50 medical mask would alleviate the panic of shortage of mask. Prior to re-use of mask,
51 we should inactivate potential contaminated virus on the mask. Heat inactivation of virus
52 such as incubating at 56°C for 30min is widely accepted to be able to inactivate
53 enveloped virus like influenza virus and coronavirus. And importantly, heating at
54 70 °C for 24 hour does not significantly change the filtration efficiency of
55 polypropylene (PP)⁶, a core matrix for medical mask, whereas conventional
56 disinfectant like ethanol dramatically destroys filter performance of polypropylene
57 electret filters⁷. We have developed a simple method to inactivate medical mask that
58 is artificially contaminated by influenza virus via heating with hair dryer for 30min
59 without affecting its filterability⁸, which can be easily adapted by public. In this study,

60 we extended our studies to optimize our protocols by shortening treatment intervals
61 with hair dryer and baking mask at different temperatures. We demonstrated that hair
62 dryer treatment for 15 min did not effectively inactivate influenza virus (IVA) on
63 medical mask compared with 30 min as described before. And that baking at 70°C for
64 30 min effectively inactivated IVA on mask whereas baking at 65°C for 30 min did
65 not. We also evaluated the filterability of mask after several-rounds of heat treatment.
66 Our results reveal that two-rounds of treatment with hair dryer for 30min or baking at
67 70°C for 30min significantly reduced filterability of mask but one-round of treatment
68 did not affect filterability of mask. Thus, we provided a simple method for reuse of
69 disposable medical mask, which may help tackle the urgent need of medical mask
70 during COVID-19 prevalence.

71

72 **Materials and Methods**

73 **Cell and virus**

74 Madin-Darby canine kidney (MDCK) cells were purchased from Cell Bank of
75 the Chinese Academy of Sciences, Shanghai, China (www.cellbank.org.cn) and
76 maintained in Dulbecco's modified medium supplemented with 10% FBS (Gibco) and
77 25mM HEPES (Gibco) with non-essential amino acids (Gibco). Influenza A(H1N1)
78 A/PR8 were purchase from ATCC and propagated in MDCK cells.

79 **Heat treatment of medical mask**

80 Medical mask was mock-contaminated by dropping a 10 μ l of IVA solution
81 containing 3.6×10^5 pfu of IVA in 3 different sites on medical mask where each site
82 was marked with a square. Due to the hydrophobic property of mask, liquid drop is
83 difficult be absorbed onto the surface of the mask. The virus drop was doted on
84 between the kink marks of the mask. Then the mask was wrapped with a food storage
85 bag and then heat treated with hair dryer (1400w, 50Hz) by moving around over the
86 surface of the wrapped mask vertically at a distance of about 10~20cm. Alternatively,
87 the wrapped mask was moved into baking oven and treated at indicated temperatures
88 with various intervals.

89 **Rescue of the virus from mask**

90 After heat treatment, the traces of IVA drop were visible within the marked
91 squares. Due to the hydrophobic property of mask, the virus within the marked
92 squares could be easily rescued by pipetting 250 μ l of Viral Transport Media (Hank's
93 Balanced Salt Solution (1X HBSS) supplemented with 0.1% bovine serum albumin
94 (BSA), 100 units/ml penicillin G and 100 units/ml streptomycin)⁹ onto the traces until

95 the traces disappear, then 125 μ l of the rescued virus was used for infecting naïve
96 MDCK cells in the presence of 5 μ g/ml TPCK-trypsin (sigma) for 1 hour at 37°C in a
97 cell culture incubator. After wash with DMEM media for 4 times, fresh DMEM media
98 with 1 μ g/ml TPCK-trypsin was added. At indicated time points post infection, the
99 supernatants were collected.

100 **Viral RNA quantification**

101 The RNAs in the supernatants from the infected MDCK cells were extracted by
102 QIAamp Viral RNA kit (Qiagen) according to the manufacturers' protocol. RNAs
103 were eluted in H₂O and quantified by a Taqman-based real time PCR with One Step
104 PrimeScript RT-PCR kit (Takara) according to the manufacturers' protocol with
105 400nM of each primer (sense primer: CTT CTA ACC GAG GTC GAA ACG TA,
106 anti-sense primer: GGT GAC AGG ATT GGT CTT GTC TTT A) and 200nM of
107 probe (FAM-TCA GGC CCC CTC AAA GCC GAG-BHQ1). The relative RNA
108 levels were calculated by 2^{- Δ CT} method ¹⁰.

109 **PM_{2.5} filterability measurement**

110 A suction flask (Shuniu, 250mL, GG-17) together with the particulate matter
111 monitor (TSI, AM510) were used to evaluate the PM_{2.5} filterability of medical masks
112 (YINUO, FE3) before and after heat treatment. Considering the effect of suction
113 process on the filtration performance of the masks, 5 experimental groups were set up
114 as following:1). Untreated group (clean unused masks without any treatment); 2).
115 One-round use + baking group (masks are used under normal condition for 4 hours
116 and then baked in oven at 70°C for 30min); 3). Two-round use+ baking group (masks

117 are used under normal condition for 8 hours, with incubation in oven at 70°C for
118 30min every 4 hours); 4). One-round use + hair dryer group (masks are used under
119 normal condition for 4 hours and then heat treated by hair dryer for 30min as
120 described above); 5). Two-round use + hair dryer group (masks are used under normal
121 condition for 8 hours, with heat treatment by air dryer for 30min every 4 hours).
122 Masks ($N=3$ /group) were tightly bound to the top of the suction flask, while the
123 particulate matter monitor was used to detect the $PM_{2.5}$ concentrations near the top
124 and the side outlet of the flask. The total suction filtration process lasted for 4 hours,
125 and the tested flow rate is 1.8 L/min. $PM_{2.5}$ concentrations were recorded every 30min,
126 and repeated for 3 times at each time point.

127

128 **Results**

129 **Heat inactivation of IVA on mock-contaminated medical mask**

130 In our previous study, baking at 56°C for 30 min only partially inactivated IVA
131 on medical mask, with a 1~3 log reduction of viral RNA level, comparing to 6 log
132 reduction of viral RNA level after hair dryer treatment for 30 min⁸. In the present
133 study, we first increased baking temperature and treated IVA mock-contaminated
134 medical mask at 65°C for 30 min. After treatment, the virus on the mask was rescued
135 and used to re-infect MDCK cells. Then we collected the supernatants of the infected
136 cells at 0 and 48 hours post infection and quantified the viral RNA levels by real-time
137 PCR. The inactivation efficiency was assessed by reduction of the viral RNA level
138 comparing to the un-treated group. Baking at 65°C for 30 min resulted in 2~5 log
139 reduction of viral RNA level but did not reduce viral RNA level to basal level (level
140 at 0 hour post infection) (Fig 1A). Hair dryer treatment for 30 min nearly completely
141 inactive IVA on medical mask⁸, while for convenience, we sought to shorten the
142 treatment intervals. We assessed the inactivation efficiency of hair dryer treatment for
143 5, 10 and 15 min as described above. As shown in Figure 1A, hair dryer treatment for
144 5, 10 and 15 min did not effectively inactive IVA.

145 Then we continued to optimize baking conditions and increase temperature to
146 70°C. We treated IVA-contaminated medical mask at 70°C for 15 min and 30 min and
147 assessed the viral replication level of the rescued virus. As shown in Figure 1B,
148 baking at 70°C for 15 min and 30 min both effectively reduced viral RNA levels to
149 nearly basal levels and treatment for 30 min was more effective than treatment for
150 15min. Thus heat treatment with hair dryer for 30min⁸ and baking at 70°C for 30 min
151 both effectively inactive IVA-contaminated medical mask.

152 **PM_{2.5} filterability of medical masks after heat treatment**

153 We assessed protective function of medical mask by measuring the filterability
154 of medical masks to ambient PM_{2.5} after similar heat treatment as described before ⁸ .
155 To evaluate the recycle times of the medical mask, masks were subjected to several
156 rounds of wear (use) and heat treatment. Masks were used under normal condition for
157 4 hours followed by treatment with hair dryer for 30min or baking at 70°C for 30 min,
158 and then subjected to a 4-hour suction process mimicking the usage scenario by an
159 adult under normal condition. As demonstrated in Figure 2A, PM_{2.5} filtration rate of
160 all the tested disposable medical masks was slightly changed during the 4-hour
161 suction process. In general, the filterability remained stable with PM_{2.5} filtration rate
162 above 85% at all the tested time points. Among all the experimental groups, masks
163 that have been used and heat treated once (by baking or hair dryer) have similar
164 4-hour average PM_{2.5} filtration rate compared to the untreated ones (Figure 2B).
165 However, after being used and heat-treated twice (by baking or hair dryer), their
166 filtration efficiency was significantly reduced as shown in Figure 2B. Our results
167 indicate that heat inactivation by baking or hair dryer for 30 min may serve as an
168 effective way for reuse of disposable medical masks, but this method is not
169 encouraged to be used for more than once.

170

171 **Discussion**

172 It is not suggested to reuse disposable medical mask, especially for people who
173 are in close contact with patients, medical staffs and laboratory technicians. But for
174 community people who are at relative low risk of contacting high dosage of
175 SARS-CoV-2, it is plausible to reuse medical mask after reliable inactivating
176 treatment during the COVID-19 prevalence, which may alleviate the heavily global
177 shortage of medical mask. We used IVA to mimic SARS-CoV-2 as they transmit
178 similarly and both have envelopes and mock contaminated medical mask by dotting
179 IVA drops onto the mask, then inactivated the IVA on medical mask by convenient
180 heat treatment with hair dryer and baking that are easily to be adapted by community
181 people. We found that baking at 70°C for 30min almost completely inactivated virus
182 as hair dryer treatment for 30min described before ⁸. But baking at 56°C and 65°C
183 for 30min could not effectively activate virus ⁸(Fig. 1A). Incubating at 56°C for
184 30min is a widely used protocol to inactivate influenza virus or coronavirus in
185 solution. The incomplete inactivation by baking at this temperature and at 65°C
186 indicates that baking a surface has less efficiency than incubating in solution.
187 Maintaining the filter function of medical mask during usage is critical for preventing
188 virus infection. We demonstrated that one-round of heat treatment did not affect
189 filterability of mask whilst two-rounds of treatment slightly but significantly reduced
190 filterability of mask. Thus, we provided a simple method for reuse of medical mask
191 by heating with hair dryer for 30min or baking at 70°C for 30min and the treated
192 mask can be reused at least once.

193 **Acknowledgements**

194 This work was inspired by professor Yuemei Wen. We are grateful to Chun-fai
195 Yung and many other colleagues for their kind suggestions and inputs. This work was
196 supported in part by the National Science and Technology Major Project of China
197 (2017ZX10103009). Key Emergency Project of Shanghai Science and Technology
198 Committee (20411950103). The funders had no role in study design, data collection
199 and analysis, decision to publish, or preparation of the manuscript.

200 **Conflict of Interest**

201 The authors declare no conflict of interest.

202

203 **Reference:**

- 204 1. Zhu N, Zhang D, Wang W, et al. A Novel Coronavirus from Patients with
205 Pneumonia in China, 2019. *The New England journal of medicine*.
206 2020;382(8):727-733.
- 207 2. Zhou P, Yang XL, Wang XG, et al. A pneumonia outbreak associated with a
208 new coronavirus of probable bat origin. *Nature*. 2020.
- 209 3. Chen L, Liu W, Zhang Q, et al. RNA based mNGS approach identifies a novel
210 human coronavirus from two individual pneumonia cases in 2019 Wuhan
211 outbreak. *Emerging microbes & infections*. 2020;9(1):313-319.
- 212 4. Li Q, Guan X, Wu P, et al. Early Transmission Dynamics in Wuhan, China, of
213 Novel Coronavirus-Infected Pneumonia. *The New England journal of*
214 *medicine*. 2020.
- 215 5. Radonovich LJ, Jr., Simberkoff MS, Bessesen MT, et al. N95 Respirators vs
216 Medical Masks for Preventing Influenza Among Health Care Personnel: A
217 Randomized Clinical Trial. *Jama*. 2019;322(9):824-833.
- 218 6. Zhang H, Liu J, Zhang X, Huang C, Jin X. Design of electret polypropylene
219 melt blown air filtration material containing nucleating agent for effective
220 PM2.5 capture. *RSC Adv*. 2018;8:7932-7941.
- 221 7. Choi H, Park E, Kim J, Kim S, Lee M. Experimental Study on Charge Decay
222 of Electret Filter Due to Organic Solvent Exposure. *Aerosol Science and*
223 *Technology*. 2015;49:977-983.
- 224 8. Song W, Pan B, Kan H, Xu Y, Yi Z. Evaluation of heat inactivation of virus

- 225 contamination on medical mask. *Journal of Microbes and Infection*.
226 2020;15(1):31-35.
- 227 9. Blachere FM, Lindsley WG, McMillen CM, et al. Assessment of influenza
228 virus exposure and recovery from contaminated surgical masks and N95
229 respirators. *Journal of virological methods*. 2018;260:98-106.
- 230 10. Livak KJ, Schmittgen TD. Analysis of relative gene expression data using
231 real-time quantitative PCR and the 2(-Delta Delta C(T)) Method. *Methods*.
232 2001;25(4):402-408.
- 233
- 234

235 **Figure Legends**

236 **Figure 1. Assessment of efficiency of heat inactivation of IVA on mask.** After
237 indicated heat treatment, IVA on the mask was rescued and used to infect naïve
238 MDCK cells. After extensive wash, the supernatants were collected at 0 and 48 hours
239 post infection (H.P.I) and the virus in the supernatants were quantified by q-PCR. The
240 RNA copy levels relative to that of the untreated (48 h) group were calculated and
241 plotted. Mean \pm SEM are shown (n=3).


242 **Figure 2. M_{2.5} filterability of disposable medical masks.** After one-round or
243 two-round use and heat treatment, the filtration rate was measured. A. PM_{2.5} filtration
244 rate change during the 4-hour suction process. * p <0.05 versus untreated group at the
245 same time point, One-way ANOVA; B. Average PM_{2.5} filtration rate within the
246 suction process were plotted. * p <0.05 versus untreated group, One-way ANOVA.
247 Mean \pm SD are shown (n=3).

248

249

250 **Figure 1**

251

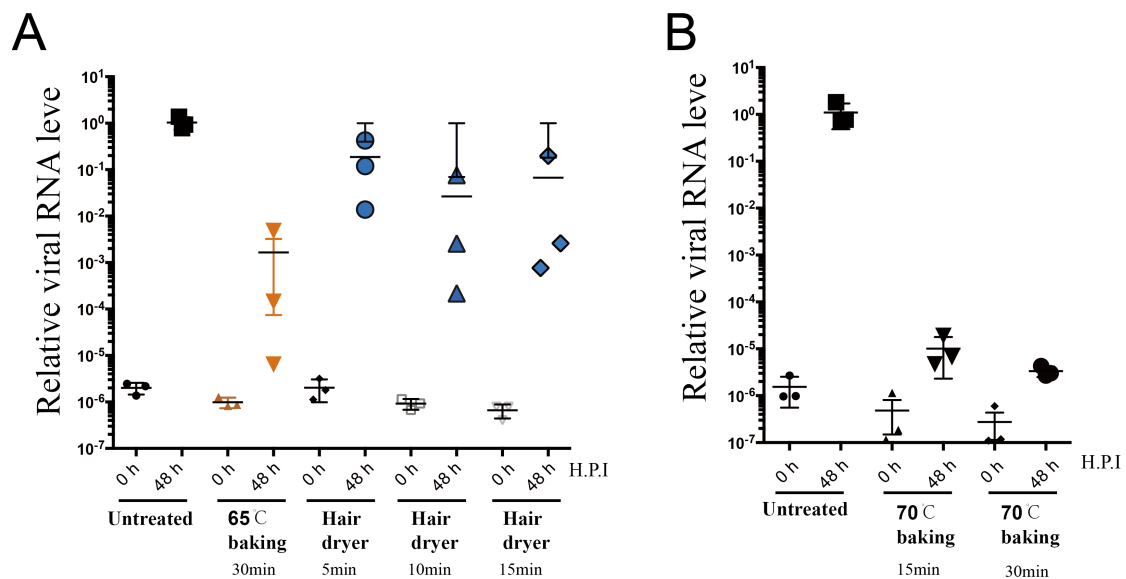

252

253 **Figure 1. Assessment of efficiency of heat inactivation of IVA on mask. After**

254 indicated heat treatment, IVA on the mask was rescued and used to infect naïve

255 MDCK cells. After extensive wash, the supernatants were collected at 0 and 48 hours

256 post infection (H.P.I) and the virus in the supernatants were quantified by q-PCR. The


257 RNA copy levels relative to that of the untreated (48 h) group were calculated and

258 plotted. Mean ± SEM are shown (n=3).

259

260 **Figure 2**

261

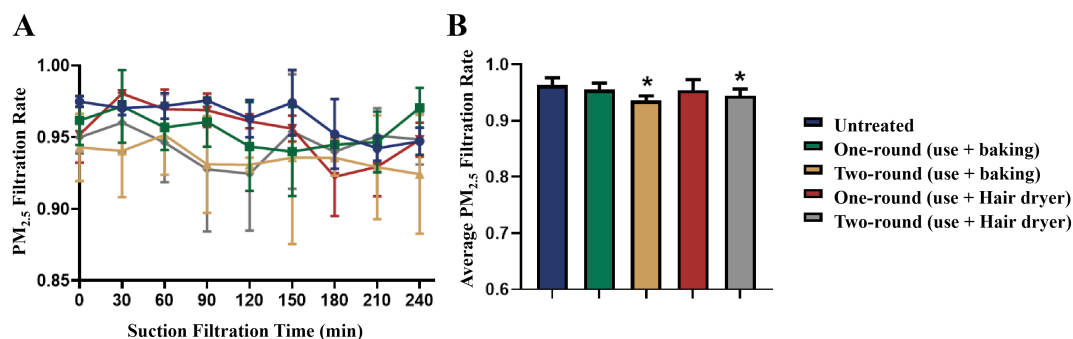

262

263 **Figure 2. PM_{2.5} filterability of disposable medical masks.** After one-round or

264 two-round use and heat treatment, the filtration rate was measured. A. PM_{2.5} filtration

265 rate change during the 4-hour suction process. * $p < 0.05$ versus untreated group at the

266 same time point, One-way ANOVA; B. Average PM_{2.5} filtration rate within the

267 suction process were plotted. * $p < 0.05$ versus untreated group, One-way ANOVA.

268 Mean \pm SD are shown (n=3).

269

270

271

272