

1 **Luminore CopperTouch™ surface coating effectively inactivates SARS-CoV-2, Ebola, and**  
2 **Marburg viruses *in vitro***

3  
4 Emily K. Mantlo<sup>a</sup>; Slobodan Paessler, DVM, PhD<sup>a</sup>; Alexey Seregin, PhD<sup>a</sup>; and Alfred Mitchell,  
5 MD<sup>b</sup>#

6  
7 <sup>a</sup> University of Texas Medical Branch, Galveston, TX, USA

8 <sup>b</sup> Luminore CopperTouch, Carlsbad, CA, USA

9  
10 Running head: Luminore CopperTouch coating inactivates viral pathogens

11  
12 # Address correspondence to:

13 Alfred Mitchell, MD

14 2060 Space Park Drive, Suite 100

15 Nassau Bay, TX, 77058

16 281-381-8576

17 [atmitchell@aol.com](mailto:atmitchell@aol.com)

18

19

20

21

22

23

24 **Abstract**

25 We investigated the ability of Luminore CopperTouch™ copper and copper-nickel  
26 surfaces to inactivate filoviruses and severe acute respiratory syndrome coronavirus 2 (SARS-  
27 CoV-2). For this purpose, we compared viral titers in Vero cells from viral droplets exposed to  
28 copper surfaces for 30 min. The copper and copper–nickel surfaces inactivated 99.9% of the viral  
29 titer of both Ebola and Marburg viruses. The copper surfaces also inactivated 99% of  
30 SARS-CoV-2 titers in 2 hours to close to the limit of detection. These data add Ebolavirus,  
31 Marburgvirus, and SARS-CoV-2 (COVID-19) to the list of pathogens that can be inactivated by  
32 exposure to copper ions, validating Luminore CopperTouch™ technology (currently the only  
33 Environmental Protection Agency-registered cold spray antimicrobial surface technology) as an  
34 efficacious, cost-friendly tool to improve infection control in hospitals, long-term care facilities,  
35 schools, hotels, buses, trains, airports, and other highly trafficked areas.

36  
37 **Keywords**

38 SARS-CoV-2 (COVID-19); Ebolavirus; Marburgvirus; filoviruses; EPA registration; copper  
39 surface; infection control; antiviral; antimicrobial; Luminore CopperTouch antimicrobial touch  
40 surfaces

41

42

43

44

45

46

## 47 **Introduction**

48 Emerging viruses continue to pose a major threat to public health worldwide, as  
49 demonstrated by two ongoing outbreaks. Recently, severe acute respiratory syndrome  
50 coronavirus 2 (SARS-CoV-2) emerged from a seafood market in Wuhan, China, and quickly  
51 spread around the world. This virus is responsible for millions of infections and over 345,523  
52 deaths worldwide and 97,948 in the USA as of May 2020. Viruses from the *Filoviridae* family  
53 have caused several outbreaks and epidemics in the past. Ebolavirus caused an outbreak of Ebola  
54 virus disease (EVD) in the West African nations of Liberia, Sierra-Leone, Guinea, Nigeria,  
55 Senegal, and Mali in 2014–2015, with a current outbreak in the Democratic Republic of the  
56 Congo (1, 2). In total, as of May 2020 at least 32,000 people have been infected and  
57 approximately 13,600 people have lost their lives due to these outbreaks. Ebolavirus and  
58 Marburgvirus, which cause hemorrhagic fevers, present a substantial global threat to public  
59 health. Reports from the World Health Organization and the Centers for Disease Control and  
60 Prevention (CDC) showed shocking fatality rates from Ebola (~70%) and Marburg hemorrhagic  
61 fever (~75%) among reported cases during 2015. As of April 2020, a total of 3462 EVD cases,  
62 including 3316 confirmed and 145 probable cases, have been reported, with a total of 2279  
63 reported deaths (overall case fatality ratio of 66%). Both Ebolavirus and Marburgvirus originated  
64 in Africa, which has experienced the bulk of outbreaks and resultant deaths, but healthcare  
65 facilities in Europe and the United States have also reported infected patients.

66 Many infectious microorganisms can survive for days or weeks after landing on a  
67 surface, presenting a tremendous challenge for infection control. In one study, Zaire Ebolavirus  
68 and Lake Victoria Marburgvirus were shown to survive in liquid media at titers above detectable  
69 limits for up to 46 days, although the number of viable particles decreased over that time (3).

70 When dried on solid surfaces, such as rubber, glass, or plastic, Ebolavirus survives at detectable  
71 levels for 5.9 (4) to 14 days (3). SARS-CoV-2 can survive on plastic or stainless steel surfaces  
72 for up to 72 h and on copper for 4 h (5). To control the spread of these infections, many  
73 guidelines and regulations have been established in hospitals, healthcare and other facilities.  
74 Healthcare authorities have instituted routine questioning of patients and visitors regarding their  
75 previous geographical location as they enter healthcare facilities  
76 (<https://www.cdc.gov/coronavirus/2019-ncov/hcp/us-healthcare-facilities.html>). Barrier nursing,  
77 characterized by isolating patients, wearing protective clothing, and disinfecting surfaces, is key  
78 to preventing the spread of both filoviruses and coronaviruses  
79 (<https://www.cdc.gov/vhf/index.html>, <https://www.cdc.gov/coronavirus/2019-ncov/hcp/infection-control-recommendations.html>). To clean healthcare facilities, the CDC  
80 requires hospital disinfectants to be effective against certain viruses with genetic structures  
81 similar to that of Ebola and coronaviruses. The United States Environmental Protection Agency  
82 (EPA) has also created a list of recommended disinfectants that are efficacious against SARS-  
83 CoV-2 ([https://www.epa.gov/pesticide-registration/list-n-disinfectants-use-against-sars-cov-2-](https://www.epa.gov/pesticide-registration/list-n-disinfectants-use-against-sars-cov-2-covid-19)  
84 [covid-19](https://www.epa.gov/pesticide-registration/list-n-disinfectants-use-against-sars-cov-2-covid-19)).

86 Commensurate with the evaluation of these preventive efforts, attention has turned to the  
87 feasibility of self-sanitizing surfaces. Copper exhibits a self-sanitizing characteristic, but its  
88 weight and bulk have limited its use. To circumvent these challenges, antimicrobial copper  
89 coatings have been developed. Luminore CopperTouch™ is an EPA-registered antimicrobial  
90 copper surface. Copper and copper–nickel formulations are currently registered and available for  
91 application in hospitals, doctor’s offices, airports, buses, trains, and other heavily trafficked  
92 areas. These antimicrobial coatings greatly expand the possibility of using copper within the

93 transportation and healthcare settings, particularly for high-touch surfaces, to reduce the spread  
94 of infection. Employing these coatings to prevent infection is preferable to attempts at treatment  
95 or curing the disease after infection occurs.

96         Several studies have demonstrated the effect of copper in reducing the bacterial burden in  
97 hospitals and healthcare facilities. Salgado *et al.* reported a significant reduction in hospital-  
98 acquired infections and/or methicillin-resistant *Staphylococcus aureus* or vancomycin-resistant  
99 *Enterococcus* colonization for patients that received treatment in intensive care unit (ICU) rooms  
100 with copper alloy surfaces compared with standard ICU rooms (6). Viruses are susceptible to  
101 copper surfaces as well, including influenza A virus (7) and norovirus (8, 9), both of which are  
102 inactivated by copper. Solid copper surfaces have also been shown to inactivate SARS-CoV-2  
103 (5).

104         Because Ebolavirus and Marburgvirus are considered biosafety level (BSL)-4 agents and  
105 SARS-CoV-2 is considered a biosafety level (BSL)-3 agent, the capacity to study these viruses is  
106 limited to specially equipped, government-registered laboratories. We investigated the effect of  
107 copper and copper–nickel surfaces on the viability of Ebolavirus and Marburgvirus. We found  
108 that these surfaces begin to inactivate the viruses within 15 min, reducing the viral load to 1%–  
109 3% of the initial titer within 30 min. These findings add Ebolavirus and Marburgvirus to the  
110 growing list of infectious microorganisms that are inactivated upon copper exposure. We also  
111 investigated the effect of Luminore CopperTouch™ copper-coated surfaces on SARS-CoV-2  
112 and observed a significant drop (99%) in viral titer after 2 hours. These findings lend strong  
113 support to the use of Luminore CopperTouch™ and other copper surfaces in hospitals, buses,  
114 trains, and public areas to reduce the spread of viral infections, with substantial implications for  
115 public health.

116

## 117 **Results**

118           Copper-coated surfaces inhibit the growth of Gram-positive and Gram-negative bacteria,  
119 as well as influenza virus, norovirus, and human immunodeficiency virus (HIV). To determine  
120 whether copper and copper–nickel surfaces can effectively reduce the viral load of Ebolavirus  
121 and Marburgvirus after exposure, 10- $\mu$ l droplets of viral suspension were exposed to Luminore  
122 CopperTouch™ surfaces for 30 min at room temperature. Marburgvirus was also tested in 10 1-  
123  $\mu$ l droplets. We measured the viral load using a standard plaque assay in Vero E6 cells. We  
124 observed a 99.9% reduction in viral titer on copper surfaces for MARV and EBOV relative to the  
125 sham surfaces after 30 min (Fig. 1), approaching the limits of assay detection. These data suggest  
126 that the CopperTouch surfaces can effectively inactivate EBOV and MARV particles.

127           To determine how rapidly copper surfaces can inactivate viral particles, we measured  
128 EBOV viral titers using plaque assays on Vero cells after viral suspensions had been exposed to  
129 surfaces for 1, 15, or 30 min (Fig. 2). At 1 and 15 min, the viral titers decreased by  
130 approximately 0.5 log-fold relative to the sham surface. After 30 min, the copper surface had  
131 reduced the viral load approximately 1.5 log-fold, corresponding to a 97% reduction in viral  
132 titers. The copper–nickel surface displayed a decrease of 2.3 log-fold, corresponding to a  
133 reduction of more than 99% in viral titers. These data suggest that viral inactivation occurs  
134 within 15–30 min and that the viral load is reduced by nearly 99% within that time period.

135           Finally, we assessed the ability of copper surfaces to inactivate SARS-CoV-2 particles.  
136 We exposed copper, metal, and plastic surfaces to SARS-CoV-2 for 2, 4, or 8 hours and  
137 measured viral titers via TCID<sub>50</sub>. Regardless of the incubation time, the copper-coated surfaces

138 reduced the viral titers greater than 2-fold, approaching the limit of detection (Fig. 3). This value  
139 corresponds to a reduction of more than 99% in viral titers.

140

## 141 **Discussion**

142 In this study, SARS-CoV-2 titers were reduced by more than 99% after 2 hours. Both  
143 MARV and EBOV viral titers were reduced by more than 99% on copper surfaces within 30  
144 min. Previous research has demonstrated that EBOV can persist on dry surfaces for 1–2 weeks  
145 (3, 4). By reducing the persistence rate, Luminore CopperTouch™ copper surfaces can shorten  
146 the viral particle survival time by up to 336-fold compared to plastic or metal surfaces. Copper-  
147 coated surfaces can also significantly reduce SARS-CoV-2 survival in comparison to plastic or  
148 metal surfaces. These findings have far-reaching implications for patient welfare and healthcare  
149 costs. Of immediate interest is the use of these coatings in healthcare, public transportation, and  
150 other settings to prevent the spread of viruses. By mitigating the presence, growth, and spread of  
151 such pathogens on frequently touched surfaces, copper coatings can play an important role in  
152 infection control and disease prevention.

153 Research on the antiviral and antibacterial properties of copper alloys and other metals  
154 (e.g., silver, iron) has increased tremendously over the past five years. Researchers have turned  
155 to self-sanitizing surfaces as a supplementary infection control strategy, given the challenges of  
156 vaccine and antibiotic development. In addition to copper, surfaces containing silver and zinc  
157 also exhibit antimicrobial properties. Sehmi *et al.* developed a method for encapsulating silicone  
158 and polyurethane with copper, which both exhibited potent bacterial activity (10). By comparing  
159 thick (100- $\mu$ m) and thin (25- $\mu$ m) rolled copper plates, researchers have noted that thin-rolled  
160 sheets are rougher in texture than thick-rolled sheets. However, the data comparing their relative

161 effectiveness are contradictory. While Zeiger *et al.* demonstrated that smoother copper surfaces  
162 have more antibacterial activity than rough surfaces (11), Yousuf *et al.* showed that thin-rolled  
163 sheets have more potent activity and attributed this effect to the increased surface area of the  
164 rough surfaces (12). More recently, a hybrid coating containing silver, copper, and zinc cations  
165 was found to significantly reduce viral titers for HIV-1, human herpesvirus 1, dengue virus type  
166 2, and influenza H1N1 virus (13). With these advancing breakthroughs in the design of self-  
167 sanitizing surfaces, our finding that Luminore CopperTouch™ copper surfaces inactivate viruses  
168 of critical public health concern adds to the enthusiasm for copper surfaces in hospitals and  
169 public spaces to aid in infection control.

170         The mechanism by which copper inactivates microorganisms is not completely  
171 understood. Winstein *et al.* demonstrated that copper can donate and accept single electrons,  
172 which produces reactive oxygen species and free radicals, causing cell death. In another study,  
173 Warnes *et al.* reported that copper surfaces inhibit the transfer of DNA (i.e., plasmids harboring  
174 antibiotic resistance mechanisms) between multidrug-resistant bacteria (14). The ability of  
175 copper to inhibit bacteria involves the rapid degradation of genomic and plasmid DNA. This  
176 study further showed that DNA degrades rapidly on copper surfaces (14). Thus, it is plausible to  
177 hypothesize that the genomes of these viruses are disrupted by the free radicals produced upon  
178 contact with copper ions.

179         In conclusion, we have shown that the copper and copper–nickel alloys produced by  
180 Luminore CopperTouch™ have a potent antiviral effect against Ebolavirus, Marburgvirus, and  
181 COVID-19. These data have significant implications for infection control, particularly during  
182 times of regional epidemics, for hospitals and other highly trafficked areas, such as doctor’s  
183 offices, prisons, airports, buses, trains, and schools. Additionally, these data could influence

184 strategies for epidemic relief for both ongoing and future epidemics, such as the current SARS-  
185 CoV-2 pandemic and the ongoing EBOV epidemic in the Democratic Republic of Congo, by  
186 supporting the use of copper coatings on equipment sent to highly affected areas.

187 **Significance and Impact.** In this study, data regarding the survival of Ebola, Marburg,  
188 and SARS-CoV-2 viruses on copper (Luminore CopperTouch™) are presented for the first time.  
189 These data will aid in the implementation of strategies to help prevent infection and transmission  
190 of disease.

191

## 192 **Materials and Methods**

### 193 *Viral strains and propagation*

194 Filoviruses were maintained in a government-registered BSL-4 facility at the University  
195 of Texas Medical Branch in Galveston, TX, in compliance with all regulations therein. Zaire  
196 ebolavirus (EBOV; Stock) and Angola Marburg virus (MARV; Stock) were utilized, and SARS-  
197 CoV-2 (USA-WA1/2020) was obtained from the World Reference Center for Emerging Viruses  
198 and Arboviruses (WRCEVA). All experiments with SARS-CoV-2 were conducted in approved  
199 BSL-3 facilities at the University of Texas Medical Branch.

### 200 *Cell culture*

201 Vero or Vero E6 cells were cultured and maintained in Eagle's minimum essential  
202 medium (MEM) with Earle's BSS (balance salt solution) and L-glutamine (EMEM) or  
203 Dulbecco's modified Eagle medium. The media were supplemented with fetal bovine serum  
204 (FBS; 1%–2%) and 100 µg/ml penicillin/streptomycin (pen/strep) solution. This same medium  
205 was used as dilution medium for plaque assays. The cells were incubated at 37±2°C with 5%  
206 CO<sub>2</sub>.

207 *Surfaces*

208 LuminOre(r) is a unique patented cold spray liquid metal. It is a polymetal alloy, not a  
209 paint. To the best of our knowledge, LuminOre is the only company that has ever been able to  
210 blend cold alloy metals and polymers together to form this type of homogeneous metal matrix.  
211 This liquid metal is then cold sprayed onto any substrate to form a solid metal surface. The  
212 Luminore CopperTouch™ copper surface is 85% copper, and the copper–nickel alloy is a  
213 proprietary blend containing 62.5% copper. For surfaces, 1-mm thick, 1 × 1-cm coupons were  
214 employed.

215 *Filovirus surface exposure*

216 The viral load consisted of 10<sup>5</sup> plaque-forming units (pfu) and viral suspensions  
217 maintained in growth medium solution (DMEM with 1x L-glutamine, 1x pen/strep, 1% MEM  
218 vitamins, and 10% FBS). Vero E6 cells were grown to 70%–80% confluence in 6- or 12-well  
219 plates. Ten 1-μl drops (MARV) or one 10-μl drop (MARV and EBOV) of viral suspensions were  
220 dispensed on either copper, copper–nickel, or sham coupons (as described above) or on uncoated  
221 metallic or plastic surfaces as controls, with a subsequent 30-min incubation at room  
222 temperature. The drops were then collected with 100 μl of fresh dilution medium and titrated on  
223 Vero E6 cells using a standard plaque assay technique (0.5% agarose overlay) (15). Inoculated  
224 Vero E6 cells were incubated at 37±2°C with 5% CO<sub>2</sub> for 7 (MARV) or 10 days (EBOV). The  
225 titrations were subsequently fixed with formalin. To enumerate the plaques, the wells were  
226 stained with neutral red or crystal violet solutions using standard procedures. To minimize the  
227 extent of work performed in the BSL-4 laboratory and the production of waste, experiments were  
228 conducted in duplicate.

229 *Coronavirus surface exposure*

230 Vero cells were grown to 85%–95% confluence in 96-well plates. One 10- $\mu$ l drop of  
231 SARS-CoV-2 stock ( $5 \times 10^5$  TCID<sub>50</sub>/mL [Tissue Culture Infectious Dose 50%/mL]) was added  
232 to copper-coated or uncoated metallic or plastic surfaces as controls and were incubated for the  
233 indicated duration at room temperature. These experiments were conducted in triplicate. The  
234 drops were collected with 90  $\mu$ l of fresh dilution medium and titrated on Vero cells using a  
235 TCID<sub>50</sub> assay.

236

### 237 **Competing Interests**

238 Dr. Mitchell is the co-founder and Medical Director of Luminore CopperTouch™.

239

### 240 **Funding**

241 This work was supported by a Luminore CopperTouch™ grant to SP (UTMB Project Number  
242 68858).

243

### 244 **Authors' Contributions**

245 SP and EKM conducted the experiments, AS assisted in the laboratory procedures and data  
246 collection, and AM led the project.

247

### 248 **Acknowledgements**

249 We thank Drs. Kenneth Plante (The World Reference Center for Emerging Viruses and  
250 Arboviruses, UTMB) and Natalie Thornburg (U.S. Centers for Disease Control and Prevention)  
251 for providing the SARS-CoV-2 stock virus. We thank Tom Valente for support, technical  
252 assistance, and funding. EKM was supported by NIH T32 training grant AI060549.

253 **References**

- 254 1. Kilianski A, Evans NG. 2015. Effectively communicating the uncertainties surrounding  
255 Ebola virus transmission. *PLOS Pathog* 11:e1005097.
- 256 2. Messaoudi I, Amarasinghe GK, Basler CF. 2015. Filovirus pathogenesis and immune  
257 evasion: Insights from Ebola virus and Marburg virus. *Nat Rev Microbiol* 13:663–676.
- 258 3. Piercy TJ, Smither SJ, Steward JA, Eastaugh L, Lever MS. 2010. The survival of  
259 filoviruses in liquids, on solid substrates and in a dynamic aerosol. *J Appl Microbiol*  
260 109:1531–1539.
- 261 4. Sagripanti J-L, Rom AM, Holland LE. 2010. Persistence in darkness of virulent  
262 alphaviruses, Ebola virus, and Lassa virus deposited on solid surfaces. *Arch Virol*  
263 155:2035–2039.
- 264 5. van Doremalen N, Bushmaker T, Morris DH, Holbrook MG, Gamble A, Williamson BN,  
265 Tamin A, Harcourt JL, Thornburg NJ, Gerber SI, Lloyd-Smith JO, de Wit E, Munster VJ.  
266 2020. Aerosol and surface stability of SARS-CoV-2 as compared with SARS-CoV-1. *N*  
267 *Engl J Med* 382:1564–1567.
- 268 6. Salgado CD, Sepkowitz KA, John JF, Cantey JR, Attaway HH, Freeman KD, Sharpe PA,  
269 Michels HT, Schmidt MG. 2013. Copper surfaces reduce the rate of healthcare-acquired  
270 infections in the intensive care unit. *Infect Control Hosp Epidemiol* 34:479–486.
- 271 7. Noyce JO, Michels H, Keevil CW. 2007. Inactivation of influenza A virus on copper  
272 versus stainless steel surfaces. *Appl Environ Microbiol* 73:2748–2750.
- 273 8. Warnes SL, Keevil CW. 2013. Inactivation of norovirus on dry copper alloy surfaces.  
274 *PLoS One* 8:e75017.
- 275 9. Warnes SL, Summersgill EN, Keevil CW. 2015. Inactivation of murine norovirus on a

- 276 range of copper alloy surfaces is accompanied by loss of capsid integrity. *Appl Environ*  
277 *Microbiol* 81:1085–1091.
- 278 10. Sehmi SK, Noimark S, Weiner J, Allan E, MacRobert AJ, Parkin IP. 2015. Potent  
279 antibacterial activity of copper embedded into silicone and polyurethane. *ACS Appl Mater*  
280 *Interfaces* 7:22807–22813.
- 281 11. Zeiger M, Solioz M, Edongué H, Arzt E, Schneider AS. 2014. Surface structure influences  
282 contact killing of bacteria by copper. *Microbiologyopen* 3:327–332.
- 283 12. Yousuf B, Ahire JJ, Dicks LMT. 2016. Understanding the antimicrobial activity behind  
284 thin- and thick-rolled copper plates. *Appl Microbiol Biotechnol* 100:5569–5580.
- 285 13. Hodek J, Zajícová V, Lovětinská-Šlamborová I, Stibor I, Müllerová J, Weber J. 2016.  
286 Protective hybrid coating containing silver, copper and zinc cations effective against  
287 human immunodeficiency virus and other enveloped viruses. *BMC Microbiol* 16 Suppl  
288 1:56.
- 289 14. Warnes SL, Highmore CJ, Keevil CW. 2012. Horizontal transfer of antibiotic resistance  
290 genes on abiotic touch surfaces: Implications for public health. *MBio* 3:e00489-12.
- 291 15. Paessler S, Huang C, Sencanski M, Veljkovic N, Perovic V, Glisic S, Veljkovic V. 2018.  
292 Ibuprofen as a template molecule for drug design against Ebola virus. *Front Biosci*  
293 23:947–953.
- 294
- 295
- 296
- 297
- 298

299 **Figure Legends**

300 **Figure 1. Ebolavirus (Zaire) and Marburg virus (Angola) are inactivated on copper and**  
301 **copper–nickel surfaces.** (A) EBOV (10- $\mu$ l drop) and (B) MARV (10- $\mu$ l drop or 10  $\times$  1- $\mu$ l drops)  
302 viruses were exposed to the indicated surfaces for 30 min and were then used to infect Vero E6  
303 cells. Standard plaque dilution assays were utilized to calculate the viral titer. The dashed  
304 horizontal lines indicate the limit of detection.

305  
306 **Figure 2. Ebolavirus is inactivated within 30 min of exposure to copper and copper–nickel**  
307 **surfaces.** Suspensions of Zaire Ebolavirus (EBOV) were exposed to each surface for the  
308 indicated amount of time, and the exposed viruses were then used to infect Vero cells. Standard  
309 plaque dilution assays were utilized to calculate the viral titer. Copper (triangle), copper–nickel  
310 (square), and sham (diamond) surfaces were compared for up to 30 min. Data are reported as the  
311 calculated average titers for treatments performed in duplicate to minimize BSL-4-level work.

312  
313 **Figure 3: SARS-CoV-2 is inactivated within 2 hours of exposure to copper-coated surfaces.**  
314 One 10- $\mu$ l drop of SARS-CoV-2 was added to the indicated surfaces for the denoted amount of  
315 time. The samples were collected with media and were used to immediately infect Vero cells for  
316 calculating the viral titer via TCID<sub>50</sub>. The data shown represent the average titers for experiments  
317 performed in triplicate. The error bars display the standard distribution, and the dotted line  
318 indicates the limit of detection.

319  
320  
321

322 **FIGURES for**  
323 **Luminore CopperTouch™ surface coating effectively inactivates SARS-CoV-2, Ebola, and**  
324 **Marburg viruses *in vitro***

325

326 Emily K. Mantlo<sup>a</sup>; Slobodan Paessler, DVM, PhD<sup>a</sup>; Alexey Seregin, PhD<sup>a</sup>; and Alfred Mitchell,

327 MD<sup>b</sup>#

328

329 <sup>a</sup> University of Texas Medical Branch, Galveston, TX, USA


330 <sup>b</sup> Luminore CopperTouch, Carlsbad, CA, USA

331

332


333

334

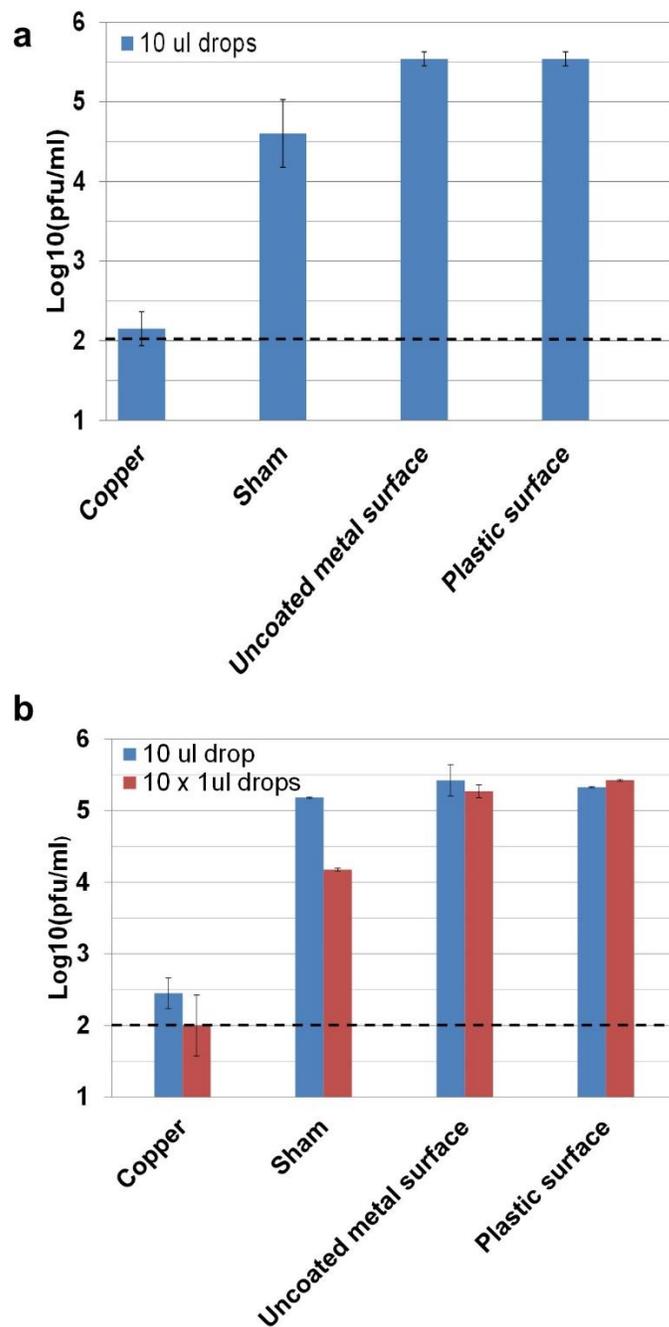


335  
336 **Figure 1. Ebolavirus (Zaire) and Marburg virus (Angola) are inactivated on copper and**  
337 **copper–nickel surfaces.** (A) EBOV (10-µl drop) and (B) MARV (10-µl drop or 10 × 1-µl drops)  
338 viruses were exposed to the indicated surfaces for 30 min and were then used to infect Vero E6  
339 cells. Standard plaque dilution assays were utilized to calculate the viral titer. The dashed  
340 horizontal lines indicate the limit of detection.

341

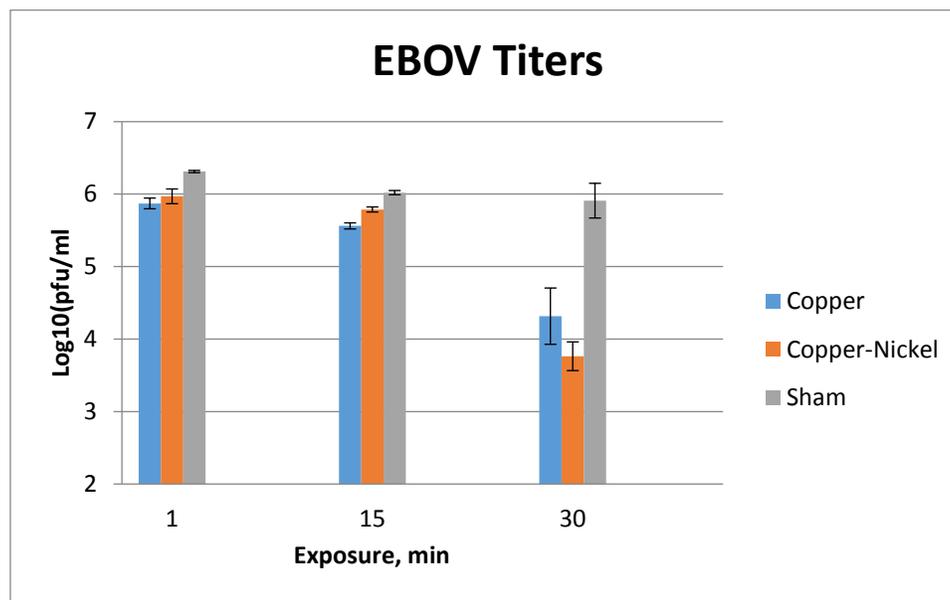

342

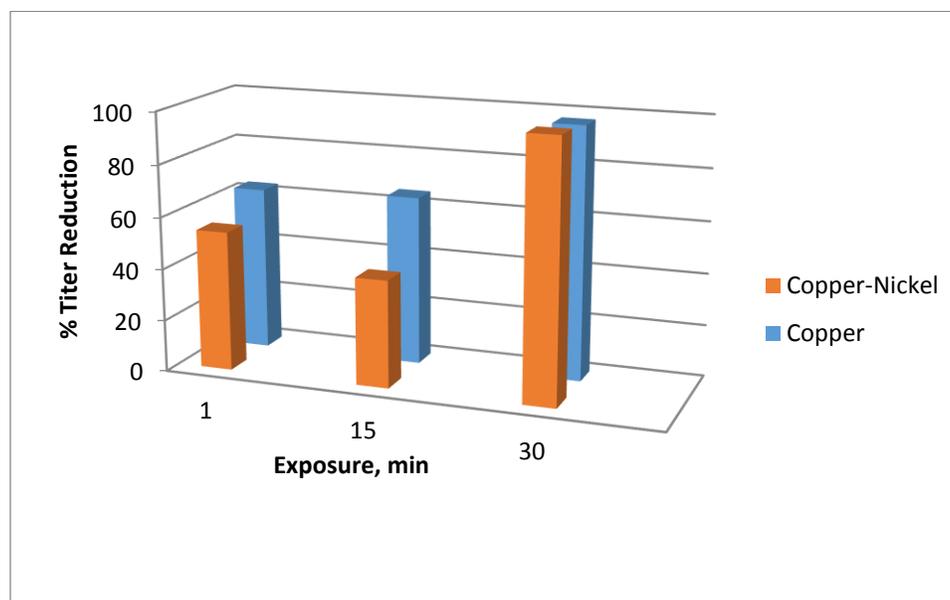


343

344 **Figure 2. Ebolavirus is inactivated within 30 min of exposure to copper and copper-nickel**  
345 **surfaces.** Suspensions of Zaire Ebolavirus (EBOV) were exposed to each surface for the  
346 indicated amount of time, and the exposed viruses were then used to infect Vero cells. Standard  
347 plaque dilution assays were utilized to calculate the viral titer. Copper, copper-nickel, and sham

348 surfaces were compared for up to 30 min. Data are reported as the calculated average titers for  
349 treatments performed in duplicate to minimize BSL-4-level work.

350  
351  
352  
353  
354  
355

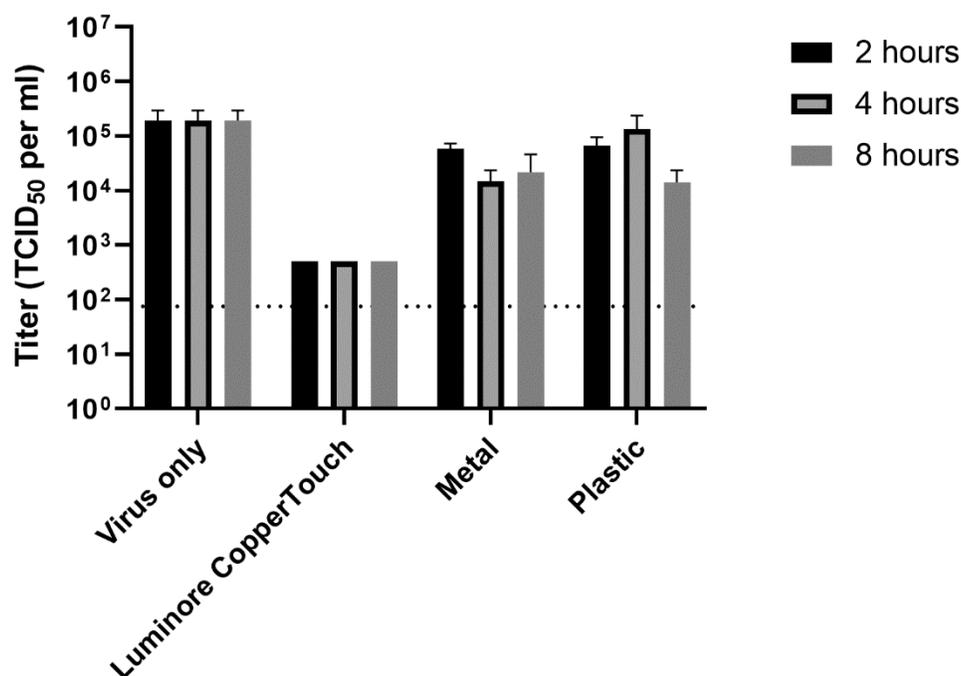

356  
357 **Figure 3: SARS-CoV-2 is inactivated within 2 hours of exposure to copper-coated surfaces.**

358 One 10- $\mu$ l drop of SARS-CoV-2 was added to the indicated surfaces for the denoted amount of  
359 time. The samples were collected with media and were used to immediately infect Vero cells for  
360 calculating the viral titer via TCID<sub>50</sub>. The data shown represent the average titers for experiments  
361 performed in triplicate. The error bars display the standard distribution, and the dotted line  
362 indicates the limit of detection.