

# **Quickly And Simply Detection For Coronavirus Including SARS-CoV-2 On The Mobile Real-Time PCR Device And Without RNA Extraction**

**Masaaki Muraoka<sup>1\*</sup>, Yukiko Tanoi<sup>1</sup>, Tetsutaro Tada<sup>1</sup>, Mikio Mizukoshi<sup>2</sup>, Osamu Kawaguchi<sup>1</sup>**

<sup>1</sup>Business Innovation Center, Nippon Sheet Glass Co. Ltd., 5-8-1, Nishi-Hashimoto, Midori-ku, Sagamihara-shi, Kanagawa, Japan

<sup>2</sup>Certified Non-Profit Organization Biomedical Science Association, 2-20-8, Kamiosaki, Shinagawa-ku, Tokyo, Japan

## **ABSTRACT**

**Severe acute respiratory syndrome coronavirus 2 (SARS-CoV-2) was reported to WHO as an outbreak in Wuhan City, Hubei Province, China on end of 2019, afterwards epidemic in many countries, and pandemic on the worldwide in 2020.**

**Usually detection of coronavirus including SARS-CoV-2 was detected by real-time RT-PCR method, but it must be long time that RNA is treated by extraction, concentration and purification, and detected by RT-PCR method. We modified various methods, of which evaluated if each method is short and simple enough.**

**In one point of the evaluations, real-time RT-PCR could be finished in very short time with using mobile real-time PCR device PCR1100 (Nippon Sheet Glass Co. Ltd.). It was able to detect positive control RNA for 20 minutes by each method according to the National Institute of Infections Disease in Japan (NIID), and less than 13.5 minutes according to the Centers for Disease Control and Prevention in USA (CDC).**

**In another point of the evaluations, surprisingly, Human coronavirus 229E, which was substituted for SARS-CoV-2, could be detected in crude state without treatment in advance of RNA. As that was, it was possible to detect coronavirus with direct RT-PCR. Therefore, it might eliminate wasteful time, avoid secondary infection and risk of contamination.**

**In light of the above two points, SARS-CoV-2 might be detected more quickly and more simply. With using this mobile real-time PCR, these methods should be suitable for not only SARS-CoV-2 but also other various viruses and might save time compared to earlier detection methods.**

\*Correspondence: [masaaki.muraoka@nsg.com](mailto:masaaki.muraoka@nsg.com)

Keywords: SARS-CoV-2, coronavirus, RNA virus real-time RT-PCR, direct RT-PCR, rapid, quick, simple, easy, mobile

## INTRODUCTION

Severe acute respiratory syndrome–coronavirus 2 (SARS-CoV-2) is a cause of coronavirus disease 2019 (COVID-19) outbreak, of which WHO declared pandemic on March 11, 2020 [1]. COVID-19 was firstly reported to WHO as an outbreak in Wuhan City, Hubei Province, China on December 31, 2019, afterwards has rapidly spreading [2]. SARS-CoV-2 included, human infectious coronaviruses have been known seven types. Four of the seven types (HCoV-229E, HCoV-HKU1, HCoV-OC43, and HCoV-NL63) are included among the known causes of common cold. Whereas, other three human coronaviruses (the Middle East respiratory syndrome coronavirus [MERS-CoV], SARS-CoV, SARS-CoV-2) are highly pathogenic and can cause severe diseases presented as acute respiratory distress syndrome (ARDS) characterized by dysfunctional immune responses and severe pulmonary injury [3] [4]. The SARS-CoV-2 virus is genetically closely related to SARS-CoV, but which is less deadly and far more transmissible than MERS-CoV or SARS-CoV [5]. Therefore, it has been needed with rapidity and on site to detect and monitor.

Routine confirmation of SARS-CoV-2 is based on detection of unique sequences of virus RNA by nucleic acid amplification tests (NAAT) such as real-time reverse-transcription polymerase chain reaction (RT-PCR). The viral genes targeted so far include the nucleocapsid (N), envelop (E), RNA-dependent RNA polymerase (RdRP), spike (S), and open reading frame 1 a/b (Orf1a/b), each of which primer and probe is various sequences [6] [7] [8] [9] [10] [11]. We recognize that the performance characteristics of PCR methods can vary with reagents, PCR programs, and devices. Therefore, if devices or reagents changed, with simpler and faster, it might be possible to detect.

And, in quantitative RT-PCR, RNA extraction is required, followed by transcription, amplification and detection. Current RT-PCR typically require more than 60 minutes for RNA extraction, concentration and purification, and a further 90 minutes for transcription and amplification [12]. It is difficult to handle RNA not to be damaged and lost, possible to infect secondary and needed long time to detect. This might be due to the delay of the initial introduction of RT-PCR detection for SARS-CoV-2 in various places.

Already reported rapid detection of SARS-CoV-2 with using mobile real-time PCR device PCR1100 [10], we suggest “simpler and faster” method of RT-PCR in this paper as follows.

## MATERIALS AND METHODS

### *Primer and Probe*

Based on previously reported protocols of NIID [6] [7] and CDC [8] [9], and detection of HCoV-229E [13], PCR primers and probes for real-time RT-PCR detection were selected to target each N gene, and synthesised (Fasmac Co. Ltd.) (Table 1.). Probe: N\_Sarbeco\_P was attached with 6-carboxyfluorescein (FAM) at the 5' end, probe: NIID\_2019-nCOV\_N\_P2 with cyan 5 (Cy5), probe: 2019-nCoV\_N1-P with FAM, probe: 2019-nCoV\_N1-P with HEX, and probe: HCoV-229E\_NP with FAM. ALL probes were attached with Black Hole Quencher (BHQ, Biosearch Technologies, Inc., USA) at the 3' end. As above, NIID version or CDC version could be used with multichannel.

### *Sample*

Positive control RNA for SARS-CoV-2 against NIID version was kindly provided from NIID (for N primer probe Ver.2 and N2 primer probe Ver.2 /Ver.3), and against CDC version were synthesised (Fasmac Co., Ltd., Japan) based on each primer sequence and information of GenBank: MN997409.1 (Table 2.). Each positive control RNA was applied 10-fold serial dilution with 10mM Tris-HCl (pH8.0 adjusted from 1M [Nippon Gene Co. Ltd., Japan] with water [UltraPure™ DNase/RNase-Free Distilled Water, Thermo Fisher Scientific Inc., USA]) included 10µg/mL carrier RNA (Ribonucleic acid from baker's yeast, Merck KGaA, Germany). And each concentration of positive control RNA was assessed relatively with detection value of PCR1100.

The above, exposure to HCoV-229E is low-risk for healthy adults. The HCoV-229E virus is easily accessible for the biosafety level 2 (BSL2) laboratory. Therefore, HCoV-229E may be a good initial model for the evaluation against other coronaviruses, such as SARS-COV-2, the coronavirus that causes COVID-19 [14]. There we substituted HCoV-229E for SARS-2-CoV in direct RT-PCR. Human coronavirus 229E (HCoV-229E, VR-740™) was bought by certified non-profit organization biomedical science association (BMSA, Japan) from American Type Culture Collection (ATCC, USA), afterwards, in cooperation of BMSA, it was able to be used. Because to proliferate HCoV-229E, it was infected with MRC-5 cells (CCL-171™, ATCC), and cultured with EMEM medium (30-2003™, ATCC) included 2% FBS (ATCC® 30-2020™) for 5~8 days in 5% CO<sub>2</sub> at 35 °C. When virus titer was grown up 8.9 x 10<sup>6</sup> Median tissue culture infectious dose (TCID<sub>50</sub>/mL), only that supernatant without MRC-5 cells was stored at -80 °C before the assay. The supernatant included HCoV-229E was thawed in the assay, not treated in advance and used with crude as it was. To assess detection value of PCR1100 relative with titer of virus, the crude sample was applied 10-fold serial dilution with 10mM Tris-HCl (pH8.0, the above).

### *Real-time RT-PCR*

RT and PCR were carrying out in the one-step with using mobile real-time PCR device PCR1100 for all tests of this study. Briefly describe the composition of RT-PCR reagent, 1 µL of a sample (the crude or positive control RNA) was amplified in a 17 µL reaction solution containing 1x Reaction Buffer, 0.25 µL of RT Enzyme Mix, 1.0 µL of DNA Polymerase (THUNDERBIRD® Probe One-step qRT-PCR Kit, TOYOBO Co. Ltd., Japan), each final concentration of primer and probe for target detection (Table 2.). With preliminary tested, each composition optimized (data not shown).

The RT-PCR conditions applied in this study were programmed as follows: RT incubation and enzyme activation were serially performed at 50 °C for 150 seconds, at 95 °C for 15 seconds respectively. Afterwards, for SARS-CoV-2 against NIID version: thermal cycling was then performed at 95 °C for 3.5 seconds (denaturation), and at 60 °C for 16 seconds (annealing and amplification) for fifty cycles. For SARS-CoV-2 against CDC version: thermal cycling was then performed at 95 °C for 3.5 seconds (denaturation), and at 60 °C for 7 seconds (annealing and amplification) for fifty cycles. For HCoV-229E: thermal cycling was then performed at 95 °C for 3.5 seconds (denaturation), and at 60 °C for 8 seconds (annealing and amplification) for fifty cycles. With preliminary tested, each condition was optimized (data not shown).

Incidentally, the procedure of PCR1100 was according to previously reported [15].

## RESULTS

### *Detection of SARS-CoV-2 in positive control RNA*

In NIID version, both No.1 and No.2 could be simultaneously detected with multichannel (Fig.1.). As the result previously reported [7], No.2 was detected more sensitive than No.1, possible to determine 10 copies too. Each Ct value (detected on the PCR1100) was depended on the rate of dilution (No.1:R<sup>2</sup>=0.9982, No.2:R<sup>2</sup>=0.9969). When simultaneously detecting with two kinds of primer / probe sets, accuracy of results could be provided with higher reliability. It took only about 20 minutes per detection on the PCR1100 with using one step RT-PCR reagent (THUNDERBIRD® Probe One-step qRT-PCR Kit). So, it could be to detect 10 copies of positive control RNA only in 20 minutes.

In CDC version, also, CDC No.1 and CDC No.2 could be detected with multichannel (Fig.2.). Both No.1 and No.2 were detected in same sensibility, and possible to detect 10 copies too. Furthermore, each Ct value (detected on the PCR1100) was depended on the rate of dilution (No.1:R<sup>2</sup>=0.9996, No.2:R<sup>2</sup>=0.9983). As the same of NIID version, when simultaneously detecting with two kinds of primer / probe sets, accuracy of results could be provided with higher reliability.

And it took only about 13.5 minutes per detection on the PCR1100 with using the same one step RT-PCR reagent, that was even faster compared with NIID version. It could detect with at least 10 copies of positive control RNA, besides it took only in 13.5 minutes.

#### *Detection of HCoV-229E in crude state*

Crude sample of HCoV-229E was applied 10-fold serial dilution, afterwards without treatment in advance and with one step RT-PCR reagent (THUNDERBIRD® Probe One-step qRT-PCR Kit) was tested in the RT-PCR on the mobile real-time PCR device PCR1100. As the result, without treatment for extraction, concentration and purification of RNA, it was possible to detect HCoV-229E at least  $8.9 \times 10^2$  TCID<sub>50</sub>/mL (Fig.3.). Furthermore, each Ct value (detected on the PCR1100) was depended on the rate of dilution, that is, virus titer ( $R^2=0.9949$ ). Ct value might be relatively indicated to virus titer.

Also, it took only about 13 minutes per detection on the PCR1100 with using one step RT-PCR reagent the same above of SARS-CoV-2. On another real-time PCR device using normal two steps RT-PCR, it needed more than 90 minutes.

Therefore, it would be able to omit more than 135 minutes (60 minutes for RNA treatment, 75 minutes for RT-PCR) in total in detection of RNA virus compared with other current methods.

## DISCUSSION

Previously reported [10] [15] [16], with using the mobile real-time PCR device PCR1100, it could be to detect unique strain rapidly, and sensibility and specificity are equivalent to other devices. But it would take 15 minutes at least to conclude RT-PCR for detection of unique RNA in any case. Furthermore, it was necessary for RNA in advance to adjust with extraction, concentration and purification.

First, this study addressed it to optimize each composition and PCR program according to previously reported [7] [10], a part of which modified to quickly carry out RT-PCR for detection of SARS-CoV-2 with using the mobile real-time PCR device PCR1100. Especially with the unit of reverse transcriptase enzyme decreased and the time of reverse transcription shorted, sensibility of detection was improved (data not shown). And, as one step RT-PCR reagent, THUNDERBIRD Probe One-step qRT-PCR Kit (TOYOBO) was used, of which was possible and efficiently to carry out RT and probe' real-time PCR simultaneously. This time, NIID and CDC version were selected for detection of SARS-CoV-2, both of which were unique for N-gene of SARS-CoV-2 and used in general [7] [8] [9]. As a result, in the NIID version No.2, CDC version No.1 and No.2, it was possible quantitatively to detect 10 copies or more of positive control RNA with using mobile real-time PCR device PCR1100. However, in the NIID, No.1 was able to detect only 100 copies or more, so No.2 was more sensitive than No.1 by 10 times. These results were about equal to previously reported [7] [10], that is, it might mean this method to be right adequate to detect positive control RNA for SARS-CoV-2. Furthermore, in both of CDC version by multichannel method, RT-PCR run could be finished in less than 14 minutes. That is, after RNA finished of extraction from each sample, this device would be quickly able to discriminate presence of target. This faster RT-PCR might be caused by combination of PCR1100 with RT-PCR reagent, of which was possible and efficiently to carry out RT and PCR simultaneously. But regretfully, in our situation unable to deal with SARS-CoV-2, this method couldn't be demonstrated possible or not for genome RNA as reported previously [7] [10]. And primer / probe sets unique for gene of SARS-CoV-2 has been variously developed till now, so we would like to investigate about those sets if RT-PCR is able to be faster to more in the PCR1100.

Second, we tried it to modify total system to detect SARS-CoV-2 easier. When treatment in advance for RNA (mainly extraction, concentration and purification) it was required more than 60 minutes [12] [13] [17]. Therefore, in this study, we tried it to carry out RT-PCR without treatment of RNA in

advance, so that, direct RT-PCR. We tested for direct RT-PCR, in that was used THUNDERBIRD® Probe One-step qRT-PCR Kit as one step RT-PCR reagent. With above, this reagent was possible and efficiently to carry out RT and probe' real-time PCR simultaneously, furthermore as reason, described possible to NAAT from crude samples [18]. And because of our situation unable to deal with SARS-CoV-2, therefore we substituted HCoV-229E, low-risk for healthy, for SARS-2-CoV in direct RT-PCR this time. As a result, surprisingly, without treatment for extraction, concentration and purification of RNA, it was possible to detect HCoV-229E at least  $8.9 \times 10^2$  TCID<sub>50</sub>/mL. Furthermore, Ct value could be relatively to virus titer. This time, Lower Limit of Detection (LoD) couldn't show accurately because failed to measure less than  $8.9 \times 10^2$  TCID<sub>50</sub>/mL. But as approximate curve shown ( $y=-4.004x+46.61$ ), the LoD is supposed to less than 1 TCID<sub>50</sub>/mL. Also, it took only about 13 minutes per detection on the PCR1100 with using one step RT-PCR reagent the same above of SARS-CoV-2. Therefore, it would be able to omit more than 135 minutes (60 minutes for RNA treatment, 75 minutes for RT-PCR) in total in detection of SARS-CoV-2 compared with other current methods. Already some reported direct RT-PCR for SARS-CoV-2, it was necessary for especial reagent and additional treatment duration to direct RT-PCR [12] [19] [20] [21] [22]. So, we could suggest novel method in this paper, in which used PCR1100 device and commercial one step RT-PCR reagent only. However, our method must be assessed in real SARS-CoV-2, further validated using clinical specimens, which contained nasopharyngeal swabs and sputum. Furthermore, real-time RT-PCR reliable in saliva reported [23] [24], its specimen must be assessed too. On the other hand, if low virus in air could be collected, it might be able to detect quickly and easily on site by our novel method, and the result be following prevent from droplet infection.

Although the other four community-acquired HCoVs (229E, OC43, HKU1, NL63) are a common cause of common cold only, they are thought to cause pandemics and major outbreaks of probably more severe respiratory diseases when they initially crossed species' barriers to infect humans decades and centuries ago [3] [25]. That is, it would be possible new coronaviruses to transfer again, therefore we are exposed to dangerous forever. On that time, the mobile real-time PCR could be it save time compared to earlier detection methods. And we think that methods suggested in this paper should be suitable for various strains and it to be useful.

## STUDY DESIGN

When each sample was assessed in the real-time RT-PCR, a ten-fold dilution series of each was indicated with high relativity to Ct value on the mobile real-time PCR device PCR1100 ( $R^2=0.99$ ).

## ACKNOWLEDGEMENTS

We thank Dr. Kazuya Shirato and Dr. Tsutomu Kageyama at the National Institute of Infections Disease in Japan (NIID) for positive control or technical comments, and Takashi Fukuzawa in an ex-employee at Nippon Sheet Glass Co. Ltd. for technical comments or experimental help.

## AUTHOR CONTRIBUTIONS

M. Muraoka conceived, designed experiments, performed experiments, analysed the data and wrote the manuscript. Y. Tanoi performed experiments and analysed the date. T. Tada wrote the manuscript. M. Mizukoshi conceived and provided specimens. O. Kawaguchi conceived, designed experiments and analysed the data. All authors also participated in the editorial process and approved the manuscript.

## ETHICAL STATEMENT

This study did not contain any studies involving human participants and animals performed by any of the authors.

## COMPETING INTERESTS

The authors declare that no competing interests exist. While M. Muraoka, T. Tanoi, T. Tada, and O. Kawaguchi were employed at Nippon Sheet Glass at the time of this study, in where all did not create a competing interest. Further, Nippon Sheet Glass had no involvement in this study.

## REFERENCES

- [1] World Health Organization (WHO) "WHO characterizes COVID-19 as a pandemic" Rolling updates on coronavirus disease (COVID-19), 11 March 2020 (<https://www.who.int/emergencies/diseases/novel-coronavirus-2019/events-as-they-happen>).
- [2] World Health Organization (WHO) "2019 Novel Coronavirus: Overview of the state of the art and outline of key knowledge gaps/slides" 12 February 2020 (<https://www.who.int/publications/m/item/2019-novel-coronavirus-overview-of-the-state-of-the-art-and-outline-of-key-knowledge-gaps-slides>).
- [3] Sin-Yee Fung, et al. "A tug-of-war between severe acute respiratory syndrome coronavirus 2 and host antiviral defence: lessons from other pathogenic viruses" *Emerg Microbes Infect.*, 2020;9(1):558-570 (<https://www.tandfonline.com/doi/full/10.1080/22221751.2020.1736644>).
- [4] Puja Mehta, et al. "COVID-19: consider cytokine storm syndromes and immunosuppression" *Lancet*, 2020;395(10229):1033–1034 ([https://www.thelancet.com/journals/lancet/article/PIIS0140-6736\(20\)30628-0/fulltext](https://www.thelancet.com/journals/lancet/article/PIIS0140-6736(20)30628-0/fulltext)).
- [5] Eskild Petersen, et al. "Comparing SARS-CoV-2 with SARS-CoV and influenza pandemics" *Lancet Infect. Dis.*, 2020;S1473-3099(20)30484-9, [Epub ahead of print] ([https://www.thelancet.com/journals/laninf/article/PIIS1473-3099\(20\)30484-9/fulltext](https://www.thelancet.com/journals/laninf/article/PIIS1473-3099(20)30484-9/fulltext)).
- [6] Victor M Corman, et al. "Detection of 2019 novel coronavirus (2019-nCoV) by real-time RT-PCR" *Euro Surveill.*, 2020;25(3):2000045 (<https://www.eurosurveillance.org/content/10.2807/1560-7917.ES.2020.25.3.2000045>).
- [7] Kazuya Shirato, et al. "Development of Genetic Diagnostic Methods for nCoV-2019 in Japan" *Jpn. J. Infect. Dis.*, 2020;73(4) [Epub ahead of print] ([https://www.jstage.jst.go.jp/article/yoken/73/4/73\\_JJID.2020.061/\\_article](https://www.jstage.jst.go.jp/article/yoken/73/4/73_JJID.2020.061/_article)).
- [8] Centers for Disease Control and Prevention "2019-Novel Coronavirus (2019-nCoV) Real-time rRT-PCR Panel Primers and Probes" 6 June 2020 (<https://www.cdc.gov/coronavirus/2019-ncov/lab/rt-pcr-panel-primer-probes.html>).
- [9] Yu Jin Jung, et al. "Comparative analysis of primer-probe sets for the laboratory confirmation of SARS-CoV-2" *bioRxiv*, 2020 (Preprint at <https://www.biorxiv.org/content/10.1101/2020.02.25.964775v1>).
- [10] Kazuya Shirato, et al. "An ultra-rapid real-time RT-PCR method using the PCR1100 to detect Severe Acute Respiratory Syndrome Coronavirus-2" *Jpn. J. Infect. Dis.*, 2020 [Epub ahead of print] ([https://www.jstage.jst.go.jp/article/yoken/advpub/0/advpub\\_JJID.2020.324/\\_article](https://www.jstage.jst.go.jp/article/yoken/advpub/0/advpub_JJID.2020.324/_article)).

- [11] World Health Organization (WHO) "Laboratory testing for 2019 novel coronavirus (2019-nCoV) in suspected human cases" 19 March 2020 (<https://www.who.int/publications/i/item/laboratory-testing-for-2019-novel-coronavirus-in-suspected-human-cases-20200117>).
- [12] Soon Keong Wee, et al. "Rapid Direct Nucleic Acid Amplification Test without RNA Extraction for SARS-CoV-2 Using a Portable PCR Thermocycler" *Genes (Basel)*, 2020, 11(6):664 (<https://www.mdpi.com/2073-4425/11/6/664>).
- [13] Leontine J R van Elden, et al. "Frequent Detection of Human Coronaviruses in Clinical Specimens from Patients with Respiratory Tract Infection by Use of a Novel Real-Time Reverse-Transcriptase Polymerase Chain Reaction" *J. Infect. Dis.*, 2004;189(4):652–657 (<https://academic.oup.com/jid/article/189/4/652/839121>).
- [14] Keykavous Parang, et al. "Comparative Antiviral Activity of Remdesivir and Anti-HIV Nucleoside Analogs Against Human Coronavirus 229E (HCoV-229E)" *Molecules*, 2020;25(10):2343 (<https://www.mdpi.com/1420-3049/25/10/2343>).
- [15] Kazuya Shirato, et al. "Ultra-Rapid Real-Time RT-PCR Method for Detecting Middle East Respiratory Syndrome Coronavirus Using a Mobile PCR Device, PCR1100" *Jpn. J. Infect. Dis.*, 2020;73(3):181-186 ([https://www.jstage.jst.go.jp/article/yoken/73/3/73\\_JJID.2019.400/article](https://www.jstage.jst.go.jp/article/yoken/73/3/73_JJID.2019.400/article)).
- [16] Kazuya Shirato, et al. "An ultra-rapid real-time RT-PCR method for detecting human orthopneumovirus using PCR1100" *Jpn. J. Infect. Dis.*, 2020 [Epub ahead of print] ([https://www.jstage.jst.go.jp/article/yoken/advpub/0/advpub\\_JJID.2020.182/article](https://www.jstage.jst.go.jp/article/yoken/advpub/0/advpub_JJID.2020.182/article)).
- [17] Centers for Disease Control and Prevention, "CDC Influenza SARS-CoV-2 (Flu SC2) Multiplex Assay" 9 July 2020 (<https://www.fda.gov/media/139743/download>).
- [18] TOYOBO Co., Ltd., Japan, "TOYOBO Life Science Raw Material Catalog ," 1 March 2019;p1 (<http://www.bio-toyobo.cn/pdf/RawMaterialCatalog.pdf>).
- [19] Emily A Bruce, et al. "DIRECT RT-qPCR DETECTION OF SARS-CoV-2 RNA FROM PATIENT NASOPHARYNGEAL SWABS WITHOUT AN RNA EXTRACTION STEP" *bioRxiv*, 2020 (Preprint at <https://www.biorxiv.org/content/10.1101/2020.03.20.001008v2>).
- [20] Licia Bordi, et al. "Rapid and sensitive detection of SARS-CoV-2 RNA using the Simplexa™ COVID-19 direct assay" *J. Clin. Virol.*, 2020;128:104416 (<https://www.sciencedirect.com/science/article/pii/S138665322030158X>)
- [21] Natacha Merindol, et al. "SARS-CoV-2 detection by direct rRT-PCR without RNA extraction" *J. Clin. Virol.*, vol. 2020;128:104423 (<https://www.sciencedirect.com/science/article/pii/S1386653220301657?via%3Dihub>)
- [22] Mohammad Rubayet Hasan, et al. "Detection of SARS-CoV-2 RNA by direct RT-qPCR on nasopharyngeal specimens without extraction of viral RNA" *PLoS One*, 2020;15(7):e0236564 (<https://journals.plos.org/plosone/article?id=10.1371/journal.pone.0236564>)

- [23] Kelvin Kai-Wang To, et al. "Consistent detection of 2019 novel coronavirus in saliva" *Clin. Infect. Dis.*, 2020;71(15):841-843 (<https://academic.oup.com/cid/article/71/15/841/5734265>)
- [24] Lorenzo Azzi, et al. "Saliva is a reliable tool to detect SARS-CoV-2" *J. Infect.*, 2020;81(1):e45-e50 ([https://www.journalofinfection.com/article/S0163-4453\(20\)30213-9/fulltext](https://www.journalofinfection.com/article/S0163-4453(20)30213-9/fulltext))
- [25] Victor M. Corman, et al. " Chapter Eight - Hosts and Sources of Endemic Human Coronaviruses " *Adv. Virus Res.*, 2018;100:163-188  
(<https://www.sciencedirect.com/science/article/pii/S0065352718300010?via%3Dihub>)

Table 1. Selected primers and probes for the real-time RT-PCR of SARS-CoV-2 NIID and CDC, and HCoV-229E

target	primer/probe	Sequence	final conc.
N_Sarbeco (NIID No.1)	N_Sarbeco_F	5'-CAC ATT GGC ACC CGC AAT C-3'	0.40μM
	N_Sarbeco_R	5'-GAG GAA CGA GAA GAG GCT TG-3'	0.60μM
	N_Sarbeco_P	5'-FAM-ACT TCC TCA AGG AAC AAC ATT GCC A-BHQ-3'	0.20μM
NIID_2019-nCoV_N2 (NIID No.2)	NIID_2019-nCoV_N_F2	5'-AAA TTT TGG GGA CCA GGA AC-3'	0.40μM
	NIID_2019-nCoV_N_R2 ver3	5'-TGG CAC CTG TGT AGG TCA AC-3'	0.60μM
	NIID_2019-nCoV_N_P2	5'-Cy5-ATG TCG CGC ATT GGC ATG GA-BHQ-3'	0.20μM
2019-nCoV_N1 (CDC No.1)	2019-nCoV_N1-F	5'-GAC CCC AAA ATC AGC GAA AT-3'	0.20μM
	2019-nCoV_N1-R	5'-TCT GGT TAC TGC CAG TTG AAT CTG-3'	0.20μM
	2019-nCoV_N1-P	5'-FAM-ACC CCG CAT TAC GTT TGG TGG ACC-BHQ-3'	0.20μM
2019-nCoV_N2 (CDC No.2)	2019-nCoV_N2-F	5'-TTA CAA ACA TTG GCC GCA AA-3'	0.40μM
	2019-nCoV_N2-R	5'-GCG CGA CAT TCC GAA GAA-3'	0.40μM
	2019-nCoV_N2-P	5'-HEX-ACA ATT TGC CCC CAG CGC TTC AG-BHQ-3'	0.20μM
HCoV-229E_N	HCoV-229E_NF	5'-CAG TCA AAT GGG CTG ATG CA-3'	0.30μM
	HCoV-229E_NR	5'-AAA GGG CTA TAA AGA GAR* TAA GGT ATT CT-3'	0.30μM
	HCoV-229E_NP	5'-FAM-CY**C TGA CGA CCA CGT TGT GGT TCA-BHQ-3'	0.20μM

\*R= A or G, \*\*Y= C or T

Table 2. Sequences of positive RNA control for the real-time RT-PCR of SARS-CoV-2 of CDC version.

2019-nCoV_N1	ACA AAC UAA AAU GUC UGA UAA UGG ACC CCA AAA UCA GCG A AA UGC ACC CCG CAU UAC GUU UGG UGG ACC CUC AGA UUC AAC UGG CAG UAA CCA GAA UGG AGA ACG CAG UGG GGC GCG AUC
2019-nCoV_N2	CUA AUC AGA CAA GGA ACU GAU UAC AAA CAU UGG CCG CAA A UU GCA CAA UUU GCC CCC AGC GCU UCA GCG UUC UUC GGA AUG UCG CGC AUU GGC AUG GAA GUC ACA CCU UC

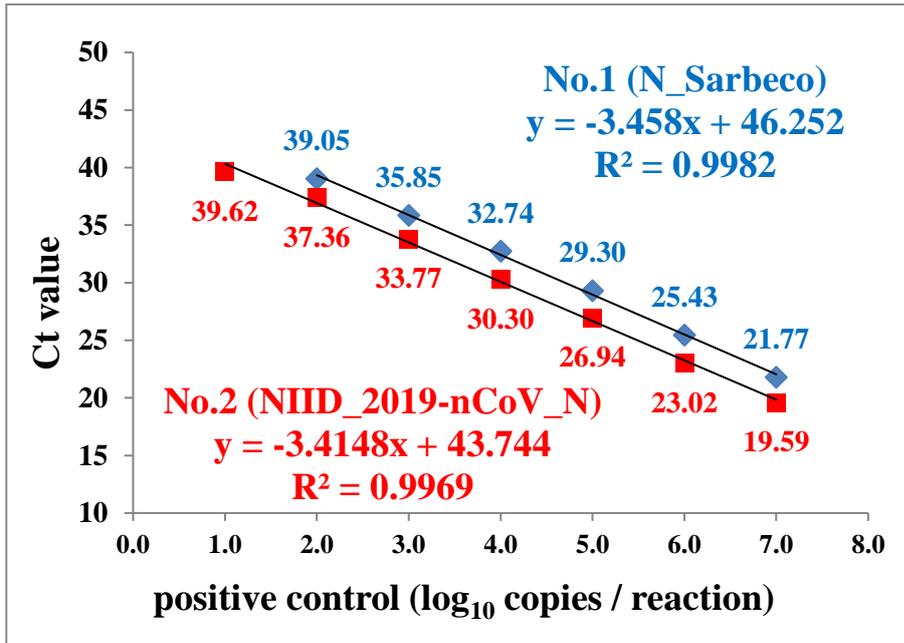


Fig.1. Correlation of copies number and Ct value when detection of positive control for NIID version on the PCR1100.

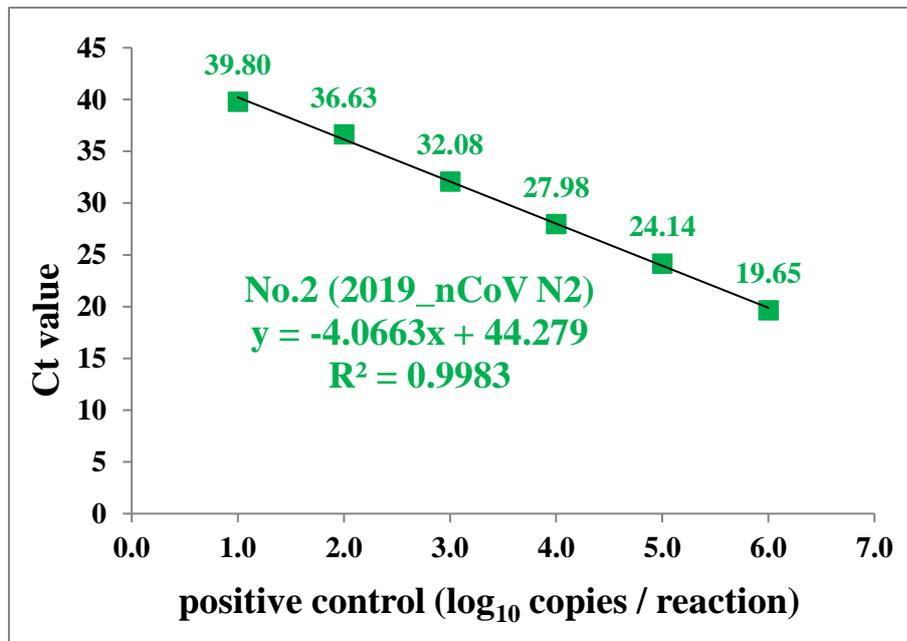
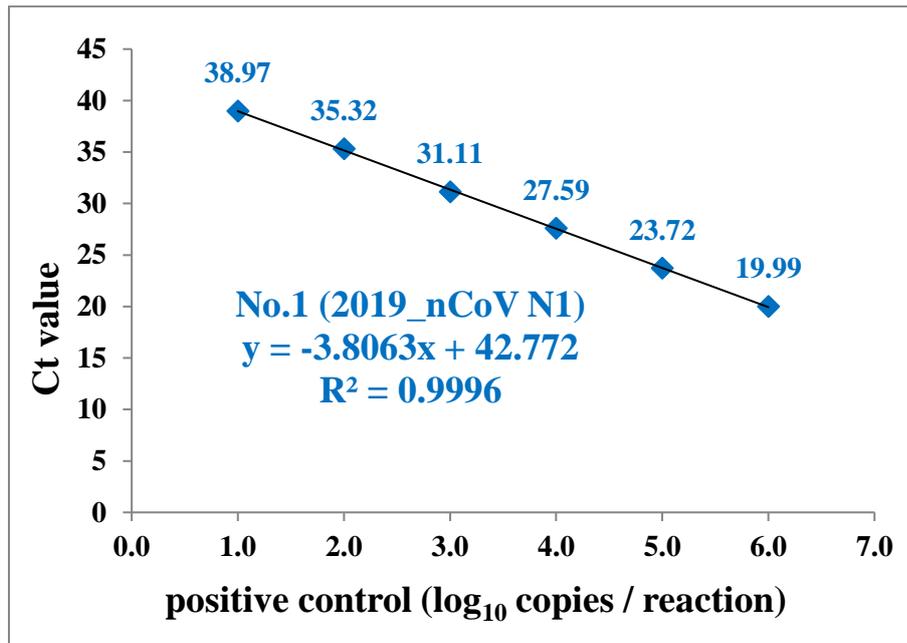


Fig.2. Correlation of copies number and Ct value when detection of positive control for CDC version on the PCR1100. The top is CDC version No.1 (2019-nCoV\_N1), the bottom is No.2 (2019-nCoV\_N2).

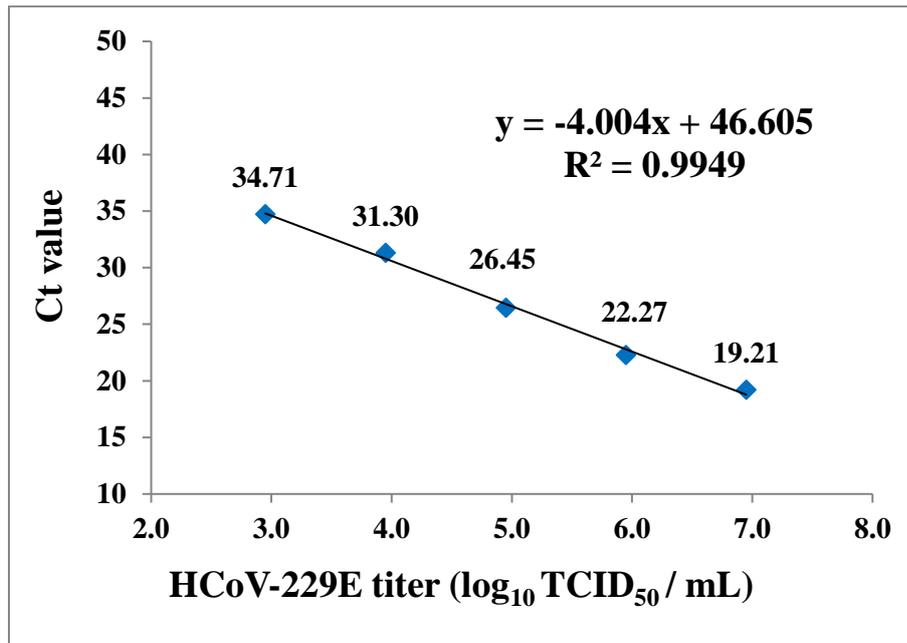


Fig.3. Correlation of virus titer and Ct value when detection of HCoV-229E on the PCR1100.