medRxiv preprint doi: https://doi.org/10.1101/2020.08.31.20185074; this version posted September 2, 2020. The copyright holder for this preprint (which was not certified by peer review) is the author/funder, who has granted medRxiv a license to display the preprint in perpetuity.
It is made available under a CC-BY-NC-ND 4.0 International license .

Fully automated detection and differentiation of pandemic and endemic coronaviruses (NL63, 229E, HKU1, OC43 and SARS-CoV-2) on the Hologic Panther Fusion

Anne Katrin Cordes,[a] William M. Rehrauer,[b] Molly A. Accola,[c] Benno Wölk,[d] Birgitta Hilfrich,[a] Albert Heim[a#]

[a]Medical School Hannover, Institute of Virology, Hannover, Germany

[b]University of Wisconsin School of Medicine and Public Health, Department of Pathology and Laboratory Medicine, Madison, Wisconsin, USA

[c]University of Wisconsin Hospital and Clinics, Molecular Diagnostics Laboratory, Madison, Wisconsin, USA

[d]LADR Medical Laboratory Dr Kramer & Colleagues, Geesthacht, Germany

running head: detection of worldwide circulating coronaviruses

address correspondence to Albert Heim, heim.albert@mh-hannover.de

NOTE: This preprint reports new research that has not been certified by peer review and should not be used to guide clinical practice.

medRxiv preprint doi: https://doi.org/10.1101/2020.08.31.20185074; this version posted September 2, 2020. The copyright holder for this preprint (which was not certified by peer review) is the author/funder, who has granted medRxiv a license to display the preprint in perpetuity.
It is made available under a CC-BY-NC-ND 4.0 International license .

Abstract

The Hologic Panther Fusion (PF) platform provides fully automated CE marked diagnostics for respiratory viruses, including recently SARS-coronavirus 2 by a transcription mediated amplification (TMA) assay, but not for the endemic human coronaviruses (hCoV). Therefore, a laboratory developed multiplexed RT-PCR protocol (LDT) that detects and differentiates the four hCoV NL63, 229E, HKU1 and OC43 was adapted on the PF.

The novel CE marked Aptima SARS-CoV-2 TMA and the LDT for hCoV were validated with 321 diagnostic specimens from the upper and lower respiratory tract in comparison to two SARS-CoV-2 RT-PCRs (PF E-gene LDT and genesig RT-PCR, 157 specimens) or the R-GENE hCoV / hParaFlu RT-PCR (164 specimens), respectively.

For the endemic hCoV, results were 96.3% concordant with two specimens discordantly positive in the PF and four specimens discordantly positive in the R-GENE assay. All discordantly positive samples had Ct values between 33 and 39. The PF hCoV LDT identified 23 hCoV positive specimens as NL63, 15 as 229E, 15 as HKU1 and 25 as OC43. The Aptima SARS-CoV-2 TMA gave 99.4 % concordant results compared to the consensus results with a single specimen discordantly positive. Moreover, 36 samples from proficiency testing panels were detected and typed correctly by both novel methods.

In conclusion, the SARS-CoV-2 TMA and the LDT for hCoV enhanced the diagnostic spectrum of the PF for all coronaviruses circulating globally for a multitude of diagnostic materials from the upper and lower respiratory tract.

medRxiv preprint doi: https://doi.org/10.1101/2020.08.31.20185074; this version posted September 2, 2020. The copyright holder for this preprint (which was not certified by peer review) is the author/funder, who has granted medRxiv a license to display the preprint in perpetuity.
It is made available under a CC-BY-NC-ND 4.0 International license .

Introduction

Human coronaviruses are a common cause for acute respiratory infections of the upper respiratory tract (1-3), though occasionally infections of the lower respiratory tract have been described. Especially children, elderly and chronically ill patients are at risk of a more severe and potentially lethal progress of disease (4-7). Four different human coronaviruses (hCoV 229E, OC43, NL63 and HKU1) are circulating in the human population worldwide. HCoV 229E and OC43 have been known since the 1960s (8, 9). More than three decades later, in 2004, the subtype NL63 (10) and in 2005 HKU1 (11) were identified. In addition to these hCoVs three zoonotic coronaviruses were discovered: SARS-CoV (causing an outbreak in 2003), MERS-CoV (discovered in 2013 and circulating almost exclusively on the Arabian Peninsula) and SARS-CoV-2 (a novel S*arbecovirus* currently pandemic and probably endemic in future). These cause severe lower respiratory tract infections in humans more frequently (12, 13). However, many SARS-CoV-2 infections can be asymptomatic or only associated with mild symptoms especially in children and young adults (14-16).

In acute respiratory infections, the rapid diagnosis of a viral etiology is essential for reducing the amount of prescribed antibiotics and for infection control measures. The introduction of nucleic acid amplification technologies (NAT) such as polymerase chain reaction (PCR) and transcription-mediated amplification (TMA) has been a milestone in the diagnosis of respiratory virus infections in comparison to virus culture and fluorescent-antibody assays improving sensitivity. Therefore, NAT is now the gold standard of coronavirus diagnostics (17, 18). However, respiratory samples are processed in batches usually once every working day for conventional coronavirus PCR diagnostics, thus resulting in long sample to answer times. Alternatively, coronavirus detection is also provided by highly multiplexed, random access PCR platforms more rapidly (19-21) but these cannot be adapted to the individual diagnostics needs of a patient considering his symptoms and the epidemiology of circulating

medRxiv preprint doi: https://doi.org/10.1101/2020.08.31.20185074; this version posted September 2, 2020. The copyright holder for this preprint (which was not certified by peer review) is the author/funder, who has granted medRxiv a license to display the preprint in perpetuity.
It is made available under a CC-BY-NC-ND 4.0 International license .

respiratory viruses. For comparison, the Hologic Panther Fusion (PF) system provides a panel of three CE marked and FDA cleared multiplex real-time PCRs that cover influenza virus A/B (Flu A/B), respiratory syncytial virus (RSV), parainfluenza virus 1-4 (ParaFlu), human metapneumovirus (hMPV), adenovirus (AdV) and rhinovirus (RhV) and can be performed according to the individual diagnostic request. These assays were validated for samples from the lower respiratory tract in a previous study (22).

Recently, a TMA based assay for SARS-CoV-2 became available for the Panther (Aptima SARS-CoV-2 assay) (23) which is CE marked and FDA cleared for emergency use (EUA) for samples from the upper respiratory tract (nasopharyngeal swabs, washes and aspirates; nasal swabs and aspirates, oropharyngeal swabs). In addition, an early laboratory developed real time PCR for the SARS-CoV E-gene (24) and a FDA EUA cleared RT-PCR for the SARS-CoV-2 Orf1ab which is only available in the U.S. (25), can be applied on the PF platform. However, the endemic human coronaviruses were not yet covered. As these are responsible for about 13-19.7 % of the respiratory infections (2, 26), we used the PF Open Access tool to establish and validate a multiplexed laboratory developed test (LDT) that detects and differentiates the four endemic hCoVs 229E, OC43, NL63 and HKU1.

medRxiv preprint doi: https://doi.org/10.1101/2020.08.31.20185074; this version posted September 2, 2020. The copyright holder for this preprint (which was not certified by peer review) is the author/funder, who has granted medRxiv a license to display the preprint in perpetuity.
It is made available under a CC-BY-NC-ND 4.0 International license .

Material and Methods

Proficiency testing panels

36 proficiency testing specimens provided by Instand (Düsseldorf, Germany) in the years 2017-2020 (sample numbers 340029 – 340050 and 340052 - 340065) were tested with the novel LDT for endemic hCoV NL63, 229E, HKU1, OC43 and the Aptima SARS-CoV-2 assay.

Panels of diagnostic specimens

In total, 321 patient samples from the upper (URT) and lower respiratory tract (LRT) were included in the panel.

164 patient samples (91 bronchial alveolar lavages (BAL), 41 nasopharyngeal swabs (NPS), 20 pharyngeal lavages (PL), 6 bronchial lavages (BL), 4 tracheal secretions (TS), 2 nasal swabs (NS)) with a diagnostic request for coronavirus were tested by the hCoV / hParaFlu R-GENE (Biomerieux, Marcy-l'Étoile, France) as the routine diagnostic procedure and the PF LDT. Specimens originated between 03/2017 and 02/2020.

For validation of the Aptima SARS-CoV-2 TMA, 157 specimens (8 BAL, 125 NPS, 1 PL, 7 BL, 3 TS, 6 NS and 7 tracheal swabs (TRS)) with a diagnostic request for SARS-CoV-2 were tested in the PF E-gene RT-PCR (24) as the routine diagnostic procedure and subsequently in the Aptima TMA and the genesig RT-PCR (Primerdesign, Chandler's Ford, UK).

Ethical statement

All 321 diagnostic samples originated from patients who had agreed to the anonymised use of their clinical data at hospital admission (informed consent). As specimens were tested according to diagnostic requests only and medical data were anonymized and analyzed only retrospectively, ethical approval is not required in Germany (confirmed by e-mails of the local

medRxiv preprint doi: https://doi.org/10.1101/2020.08.31.20185074; this version posted September 2, 2020. The copyright holder for this preprint (which was not certified by peer review) is the author/funder, who has granted medRxiv a license to display the preprint in perpetuity.
It is made available under a CC-BY-NC-ND 4.0 International license .

ethical committee "Ethikkommission der Medizinischen Hochschule Hannover", 19th of September, 2019 and 6th of May 2020).

Sample preparation

Swabs were re-suspended in 1.5 ml PBS^-. Liquid samples (lavages and secretions) were loaded without prior processing of the sample. However, viscous samples were diluted 1:2 in PBS^- to avoid clotting in the pipette tip. For testing on the PF, 500 µl of the specimen (patient specimen and proficiency testing samples) were transferred into a Specimen Lysis Tube (SLT) that contained 710 µl Specimen Transport Media (STM).

Coronavirus (NL63, 229E, HKU1 and OC43) LDT

SLTs were automatically processed on the Panther Fusion system including nucleic acid extraction, reverse transcription and real time PCR using the Open Access RNA/DNA enzyme cartridge, the Extraction Reagent-S, the Capture Reagent-S, the Enhancer Reagent-S, the internal control and the primer and probe recon solution (PPR). The PPR (table 1) contained coronavirus specific (targeting the respective N gene) as well as internal control (IC) primers and probes, $MgCl_2$, KCl, Tris buffer and nuclease free water (all ThermoFisher, Waltham, MA, USA). Coronavirus specific primer and probe sequences were published recently (27) but were labelled with different fluorescent dyes (supplementary table 1). Stability of the PPR on the Panther Fusion was validated for a period of 14 days (supplementary table 2).

Settings in the PF software for automatic processing were: extraction volume 360 µl and "sample aspiration height" low. The reverse transcription was performed at 50 °C for 8:28 minutes followed by the activation of the Taq polymerase at 95 °C for 2:00 minutes. The two step thermocycling protocol consisted of 45 cycles each with a denaturation at 95 °C for 5 seconds and the elongation and fluorescence detection at 60 °C for 22 seconds. Fluorescence

medRxiv preprint doi: https://doi.org/10.1101/2020.08.31.20185074; this version posted September 2, 2020. The copyright holder for this preprint (which was not certified by peer review) is the author/funder, who has granted medRxiv a license to display the preprint in perpetuity.
It is made available under a CC-BY-NC-ND 4.0 International license .

analysis settings in the PF software were set as following: The analysis start cycle was set at 10, the baseline correction was enabled and the slope limit was set at 25. As a positivity criteria the Ct threshold in the channels 1 (FAM for 229E), 2 (HEX for NL63) and 3 (ROX for HKU1) was set to 200 RFU, in channel 4 (Quasar 670 for OC43) to 300 RFU and in channel 5 (Quasar 705 for IC) to 1000 RFU. The crosstalk correction was set to 1 % for the combination of emitter channel 1 and receiver channel 2, as well as the combination of emitter channel 5 and receiver channel 4. A result was defined as valid if at least one positive result in channels 1-5 was detected.

Aptima SARS-CoV-2 TMA

SLTs were loaded on the Panther Fusion and the assay was performed automatically as described in the package insert (23).

SARS-CoV-2 E gene RT-PCR

The SARS-CoV-2 E gene RT-PCR was performed with the Open Access tool on the Panther Fusion as described previously (24).

HCoV/hParaFlu R-GENE RT-PCR

Nucleic acid extraction was performed on a QIAcube using the DNeasy blood kit (QIAGEN, Hilden, Germany). Of the eluate, 10 µl were tested by the hCoV / hParaFlu R-GENE assay (bioMérieux, Marcy-l'Étoile, France) on an ABI 7500 sequence detection system (ABI, Foster City, CA, U.S.). This assay has been validated previously for multiple types of respiratory specimens.

Genesig SARS-CoV-2 RT-PCR

Nucleic acid extraction was performed on a QIAcube using the DNeasy blood kit (QIAGEN, Hilden, Germany). Of the eluate, 10 µL were tested by the genesig coronavirus COVID-19

medRxiv preprint doi: https://doi.org/10.1101/2020.08.31.20185074; this version posted September 2, 2020. The copyright holder for this preprint (which was not certified by peer review) is the author/funder, who has granted medRxiv a license to display the preprint in perpetuity.
It is made available under a CC-BY-NC-ND 4.0 International license .

Real-Time PCR assay (Primerdesign, Chandler's Ford, UK) on an ABI 7500 sequence detection system.

Amplification efficiency and evaluation of LOD

The amplification efficiency was calculated from serial dilutions of reference samples if available. Supernatants from cell cultures, positive for 229E, NL63 and OC43 were provided by the national reference centre for coronaviruses at Charité, Berlin. For SARS-CoV-2, quantified quality control material "AccuPlex SARS-CoV-2 Verification panel, cat # 0505-0129" from Seracare (Milford, MA, U.S.) was used. For HKU1, no cell culture supernatant was available. Therefore, a patient sample that had been tested highly positive in the hCoV / ParaFlu R-GENE assay was used for estimating the amplification efficiency.

For the Aptima SARS-CoV-2, the limit of detection (LOD) was determined from half logarithmic serial dilutions.

Data analysis and statistics

The amplification efficiency was calculated with the following formula: Amplification efficiency (E) = $10^{-1/m}$ (with m being the slope of the amplification curve). For the Aptima SARS-CoV-2 TMA assay the LOD (95% probability of detection according to 2002/364/EC) was calculated by probit analysis from 27 replicates of a dilution series of the Accuplex standard using the statistics program SSPS (Version 15.0). For panels of diagnostic specimens, concordances of assays and positive percent agreement (PPA) and negative percent agreement (NPA) of PF assays were calculated. To evaluate the clinical performance of the Aptima SARS-CoV-2 TMA compared to those of the two other RT-PCRs (Panther Fusion E-gene LDT and genesig COVID-19 RT-PCR), a consensus result was defined as a concordant result in at least two of three tests.

medRxiv preprint doi: https://doi.org/10.1101/2020.08.31.20185074; this version posted September 2, 2020. The copyright holder for this preprint (which was not certified by peer review) is the author/funder, who has granted medRxiv a license to display the preprint in perpetuity.
It is made available under a CC-BY-NC-ND 4.0 International license .

Results

Amplification efficiencies and LOD

The LOD of the Aptima SARS-CoV-2 TMA was 288 copies/ml (95 % confidence interval 191 – 755 copies/ml) determined as the 95 % probability of detection. In case of 229E, NL63, OC43 and HKU1 the LODs were not determined due to the limited availability of quantified reference materials but amplification efficiencies of PCR were calculated. Amplification efficiencies for 229E, NL63, OC43 and HKU1 were 1.89, 1.92, 2.0 and 1.95, respectively (figure 1). For SARS-CoV-2 an amplification efficiency cannot be calculated because this assay uses TMA technology with subsequent hybridization to a SARS-CoV-2 specific probe.

Proficiency testing panel specimens and cross-reactivity

36 proficiency testing specimens provided by Instand (Düsseldorf, Germany) were tested with the hCoV LDT and Aptima SARS-CoV-2 TMA. All samples were detected correctly. From these samples, 31 were coronavirus positive samples (10 OC43, 3 NL63 and 4 229E, 4 SARS-CoV-2, 10 MERS-CoV) and 5 were negative for these coronaviruses. As anticipated, MERS-CoV positive specimens were negative in the hCoV LDT and the Aptima SARS-CoV-2 TMA. Hence, cross-reactivity with MERS-CoV could be excluded. Furthermore, an inactivated SARS-CoV positive cell culture supernatant originating from 2003 gave a negative result in the Aptima SARS-CoV-2 TMA.

Comparison of test performance for Coronavirus NL63, 229E, HKU1 and OC43 detection

A panel of 164 archived diagnostic specimens was tested with the Coronavirus LDT on the Panther Fusion and results were compared to the initial results of the hCoV / ParaFlu R-GENE assay (table 2). Overall, the concordance of results was 96.3 %. The positive percent agreement (PPA) of the LDT on the Panther Fusion was determined as 94.9 % and the

medRxiv preprint doi: https://doi.org/10.1101/2020.08.31.20185074; this version posted September 2, 2020. The copyright holder for this preprint (which was not certified by peer review) is the author/funder, who has granted medRxiv a license to display the preprint in perpetuity.
It is made available under a CC-BY-NC-ND 4.0 International license .

negative percent agreement (NPA) as 97.6 % in relation to the R-GENE assay. Samples with discordant results had Ct values of 33, 34, 36 and 39 in the R-GENE assay and 38 (two samples) in the PF LDT. In contrast to the R-GENE assay, the PF LDT provided differentiation of hCoV samples: 25 of 77 were identified as OC43, 23 as NL63, 15 as 229E and 15 as HKU1. Among these, one sample was co-infected with 229E (with a Ct value of 21) and OC43 (Ct value 32).

Diagnostic performance of the Aptima SARS-CoV-2 TMA

Of 157 samples tested, 56 were found to be consensus positive for SARS-CoV-2 RNA in any two of the tree methods (table 3). Thus, the PPA of the Aptima SARS-CoV-2 TMA and of the PF E-gene RT-PCR were determined as 100.0 % and the NPA as 99.0 %, whereas the genesig COVID-19 PCR had a PPA of 87.5 % and a NPA of 100 % (table 3). In the LDT SARS-CoV-2 RT-PCR the median Ct of positive samples was 34.2 (range 17.5 – 40.8) with an interquartile range of 6.4 and in the genesig RT-PCR the median Ct was 32.7 (range 19.2 – 39.2) and the inter quartile range 6.4. Thus the Aptima SARS-CoV-2 TMA detected multiple faintly positive samples correctly. Moreover, 23 of 157 samples originated from the lower respiratory tract and were all detected correctly in the Aptima in comparison to the consensus result with 15 of these positive for SARS-CoV-2 RNA. Detailed results for various diagnostic materials are presented in supplementary table 3.

medRxiv preprint doi: https://doi.org/10.1101/2020.08.31.20185074; this version posted September 2, 2020. The copyright holder for this preprint (which was not certified by peer review) is the author/funder, who has granted medRxiv a license to display the preprint in perpetuity.
It is made available under a CC-BY-NC-ND 4.0 International license .

Discussion

Rapid diagnostics of respiratory virus infections is essential for a quick therapeutic response as well as for complying hygiene regulations. To optimise the sample-to-answer time, the PF platform provides random access testing instead of batch-wise testing as in the hCoV / hParaFlu R-GENE assay and the genesig COVID-19 RT-PCR. Previously, only assays for influenza virus A/B, respiratory syncytial virus, parainfluenza virus 1-4, human metapneumovirus, adenovirus and rhinovirus were available for the PF. Due to the SARS-CoV-2 pandemic, a LDT for the E-gene of SARS-CoV-2 was rapidly established for the open access capability of the PF (24). Recently, a CE marked and FDA cleared SARS-CoV-2 TMA, which provides dual target detection and a high analytical sensitivity (low LOD) became available (Aptima SARS-CoV-2) (28, 29).

We evaluated the Aptima SARS-CoV-2 assay with a panel of 157 archived diagnostic specimens which included a multitude of diagnostic materials from the upper and lower respiratory tract. Although the intended use of the Aptima SARS-CoV-2 is limited to diagnostic materials from the upper respiratory tract, SARS-CoV-2 RNA was detected with 100 % PPA and 99.0 % NPA. These results compared favorably to other studies, which had only included nasopharyngeal swabs (94.7 % to 100 % PPA and 98.7 % to 100 % NPA) (28-30). However, detection of SARS-CoV-2 in materials from the LRT is crucial as it was shown that nasopharyngeal swabs may turn negative in the course of infection prior to specimens from the LRT (16, 31-33). Only a single sample gave a discordant (false positive) result in the Aptima SARS-CoV-2 assay in comparison to the consensus results. However, this sample was a follow up sample from a patient who was diagnosed as SARS-CoV-2 RNA positive in previous samples. Therefore, the Aptima SARS-CoV-2 assay may have still detected residual SARS-CoV-2 RNA due to its very low LOD. In our hands, LOD was determined to be 288 copies/ml, whereas others had a 100 % detection rate at 83 copies/ml also using quality

medRxiv preprint doi: https://doi.org/10.1101/2020.08.31.20185074; this version posted September 2, 2020. The copyright holder for this preprint (which was not certified by peer review) is the author/funder, who has granted medRxiv a license to display the preprint in perpetuity.
It is made available under a CC-BY-NC-ND 4.0 International license .

control material from Seracare but with only 20 replicates tested (29). Nevertheless, the LOD of the Aptima SARS-CoV-2 assay was even lower than the LOD of the E-gene RT-PCR on the PF (315 copies/ml). Both assays, run automatized on the PF from samples that have been processed identically before having been loaded onto the platform. On the PF, 360 µl of the sample are pipetted for both assays, however, only 10 % of the extracted nucleic acid is used for the PCR reaction, while in the TMA the total volume is applied. Although highly sensitive, the Aptima SARS-CoV-2 assay is highly specific and does not cross-react SARS-CoV (of 2003), MERS-CoV and the endemic human CoV (29), which was confirmed in our study by testing proficiency panel specimens. Previously, cross reactivity with other respiratory viruses was excluded extensively (29).

Diagnosis of endemic hCoV infections is not only required in URT infections but also in more severe LRT infections as e.g. bronchiolitis (5-7). For example, hCoV NL63 binds to the same cellular receptor as SARS-CoV-2 (34) and can be associated with severe LRT infections (10, 35). Therefore, rapid diagnosis of hCoV infections is essential and can be achieved with the novel hCoV LDT on the PF. Furthermore, a potential cross immunity to SARS-CoV-2 infection following infection with hCoV was suggested (36). Therefore, detection and classification of hCoV might be of importance in the future, to predict the prognosis of SARS-CoV-2 infection. The analysis of 164 diagnostic hCoV specimens from the upper and lower respiratory tract showed a PPA of 94.9 % and a NPA of 97.6 % compared to the results of the manual R-GENE RT-PCR. Unfortunately, a precise LOD could not be determined for the PF LDT due to a lack of quantified reference materials but the high amplification efficiencies of the PF LDT indeed suggested low LODs. This may also be supported by our diagnostic experience with the PF LDT in the winter season 2019/2020. 87 of 1732 diagnostic specimens were tested positive for endemic coronaviruses in the PF LDT. HCoV HKU1 predominated in this season (71 out of 87 coronavirus positive specimens). Other positive specimens were distributed as following: NL63 10 positives, 229E 4 positives and OC43 2

medRxiv preprint doi: https://doi.org/10.1101/2020.08.31.20185074; this version posted September 2, 2020. The copyright holder for this preprint (which was not certified by peer review) is the author/funder, who has granted medRxiv a license to display the preprint in perpetuity.
It is made available under a CC-BY-NC-ND 4.0 International license .

positives. Another limitation of the study was that HKU1 was not included in the panel of proficiency testing specimens probably because HKU1 cannot be grown in cell culture easily (37). As the R-GENE assay does not differentiate the endemic hCoV, we could not confirm that a sample positive for HKU1 in the PF LDT truly contains HKU1 RNA but 13 of 15 samples positive for HKU1 were at least confirmed as hCoV positive in the R-GENE assay. Moreover, the primer and probe sequences for HKU1 (and all other hCoVs) that had previously been published (27) were reanalyzed on specificity using Nucleotide Blast (NCBI PubMed). As no homology of the primer and probe sequences with another than the intended corresponding hCoV sequence was detected, we presume classification to be correct.

A fast and accurate differentiation of respiratory pathogens in patients with respiratory symptoms is essential to enable sufficient infectious control measures, particularly with regard to the current SARS-CoV-2 pandemic. Together with the PF respiratory panel, 15 different respiratory viruses (Flu A/B, RSV, ParaFlu 1-4, hMPV, AdV, RhV, hCoV NL63/229E/HKU1/OC43 and SARS-CoV-2) can be detected within 4 hours from one single specimen loaded on the PF. Alternatively, a cost saving step by step diagnostic approach is feasible on the PF, e.g. starting with SARS-CoV-2 testing and if negative, testing for other respiratory viruses subsequently.

Acknowledgements

We want to thank Prof. Annemarie Berger (Institute für Medizinische Virologie, Universitätsklinikum Frankfurt, Germany) for providing us SARS-CoV-1 cell culture supernatants and Dr. Victor Corman (National Reference Laboratory for Corona Viruses, Charité, Berlin) for providing us hCoV NL63, OC43 and 229E cell culture supernatants.

medRxiv preprint doi: https://doi.org/10.1101/2020.08.31.20185074; this version posted September 2, 2020. The copyright holder for this preprint (which was not certified by peer review) is the author/funder, who has granted medRxiv a license to display the preprint in perpetuity.
It is made available under a CC-BY-NC-ND 4.0 International license .

References

1. Bradburne AF, Bynoe ML, Tyrrell DA. 1967. Effects of a "new" human respiratory virus in volunteers. Br Med J 3:767-769.
2. Szilagyi PG, Blumkin A, Treanor JJ, Gallivan S, Albertin C, Lofthus GK, Schnabel KC, Donahue JG, Thompson MG, Shay DK. 2016. Incidence and viral aetiologies of acute respiratory illnesses (ARIs) in the United States: a population-based study. Epidemiol Infect 144:2077-2086.
3. Taylor S, Lopez P, Weckx L, Borja-Tabora C, Ulloa-Gutierrez R, Lazcano-Ponce E, Kerdpanich A, Angel Rodriguez Weber M, Mascarenas de Los Santos A, Tinoco JC, Safadi MA, Lim FS, Hernandez-de Mezerville M, Faingezicht I, Cruz-Valdez A, Feng Y, Li P, Durviaux S, Haars G, Roy-Ghanta S, Vaughn DW, Nolan T. 2017. Respiratory viruses and influenza-like illness: Epidemiology and outcomes in children aged 6 months to 10 years in a multi-country population sample. J Infect 74:29-41.
4. McIntosh K, Chao RK, Krause HE, Wasil R, Mocega HE, Mufson MA. 1974. Coronavirus infection in acute lower respiratory tract disease of infants. J Infect Dis 130:502-507.
5. Mayer K, Nellessen C, Hahn-Ast C, Schumacher M, Pietzonka S, Eis-Hübinger AM, Drosten C, Brossart P, Wolf D. 2016. Fatal outcome of human coronavirus NL63 infection despite successful viral elimination by IFN-alpha in a patient with newly diagnosed ALL. Eur J Haematol 97:208-210.
6. Ogimi C, Waghmare AA, Kuypers JM, Xie H, Yeung CC, Leisenring WM, Seo S, Choi SM, Jerome KR, Englund JA, Boeckh M. 2017. Clinical Significance of Human Coronavirus in Bronchoalveolar Lavage Samples From Hematopoietic Cell Transplant Recipients and Patients With Hematologic Malignancies. Clin Infect Dis 64:1532-1539.
7. Uhlenhaut C, Cohen JI, Pavletic S, Illei G, Gea-Banacloche JC, Abu-Asab M, Krogmann T, Gubareva L, McClenahan S, Krause PR. 2012. Use of a novel virus detection assay to identify coronavirus HKU1 in the lungs of a hematopoietic stem cell transplant recipient with fatal pneumonia. Transpl Infect Dis 14:79-85.
8. Hamre D, Procknow JJ. 1966. A new virus isolated from the human respiratory tract. Proc Soc Exp Biol Med 121:190-193.
9. McIntosh K, Dees JH, Becker WB, Kapikian AZ, Chanock RM. 1967. Recovery in tracheal organ cultures of novel viruses from patients with respiratory disease. Proc Natl Acad Sci U S A 57:933-940.
10. van der Hoek L, Pyrc K, Jebbink MF, Vermeulen-Oost W, Berkhout RJM, Wolthers KC, Wertheim-van Dillen PME, Kaandorp J, Spaargaren J, Berkhout B. 2004. Identification of a new human coronavirus. Nature Medicine 10:368-373.
11. Woo PC, Lau SK, Chu CM, Chan KH, Tsoi HW, Huang Y, Wong BH, Poon RW, Cai JJ, Luk WK, Poon LL, Wong SS, Guan Y, Peiris JS, Yuen KY. 2005. Characterization and complete genome sequence of a novel coronavirus, coronavirus HKU1, from patients with pneumonia. J Virol 79:884-895.
12. Drosten C, Gunther S, Preiser W, van der Werf S, Brodt HR, Becker S, Rabenau H, Panning M, Kolesnikova L, Fouchier RA, Berger A, Burguiere AM, Cinatl J, Eickmann M, Escriou N, Grywna K, Kramme S, Manuguerra JC, Muller S, Rickerts V, Sturmer M, Vieth S, Klenk HD, Osterhaus AD, Schmitz H, Doerr HW. 2003. Identification of a novel coronavirus in patients with severe acute respiratory syndrome. N Engl J Med 348:1967-1976.
13. Bermingham A, Chand MA, Brown CS, Aarons E, Tong C, Langrish C, Hoschler K, Brown K, Galiano M, Myers R, Pebody RG, Green HK, Boddington NL, Gopal R, Price N, Newsholme W, Drosten C, Fouchier RA, Zambon M. 2012. Severe respiratory illness caused by a novel coronavirus, in a patient transferred to the United Kingdom from the Middle East, September 2012. Euro Surveill 17:20290.

medRxiv preprint doi: https://doi.org/10.1101/2020.08.31.20185074; this version posted September 2, 2020. The copyright holder for this preprint (which was not certified by peer review) is the author/funder, who has granted medRxiv a license to display the preprint in perpetuity.
It is made available under a CC-BY-NC-ND 4.0 International license .

14. Chau NVV, Thanh Lam V, Thanh Dung N, Yen LM, Minh NNQ, Hung LM, Ngoc NM, Dung NT, Man DNH, Nguyet LA, Nhat LTH, Nhu LNT, Ny NTH, Hong NTT, Kestelyn E, Dung NTP, Xuan TC, Hien TT, Thanh Phong N, Tu TNH, Geskus RB, Thanh TT, Thanh Truong N, Binh NT, Thuong TC, Thwaites G, Tan LV. 2020. The natural history and transmission potential of asymptomatic SARS-CoV-2 infection. Clin Infect Dis doi:10.1093/cid/ciaa711.
15. Dong Y, Mo X, Hu Y, Qi X, Jiang F, Jiang Z, Tong S. 2020. Epidemiology of COVID-19 Among Children in China. Pediatrics 145.
16. Woelfel R, Corman VM, Guggemos W, Seilmaier M, Zange S, Mueller MA, Niemeyer D, Vollmar P, Rothe C, Hoelscher M, Bleicker T, Bruenink S, Schneider J, Ehmann R, Zwirglmaier K, Drosten C, Wendtner C. 2020. Clinical presentation and virological assessment of hospitalized cases of coronavirus disease 2019 in a travel-associated transmission cluster. medRxiv doi:10.1101/2020.03.05.20030502:2020.2003.2005.20030502.
17. Kuypers J, Wright N, Ferrenberg J, Huang ML, Cent A, Corey L, Morrow R. 2006. Comparison of real-time PCR assays with fluorescent-antibody assays for diagnosis of respiratory virus infections in children. J Clin Microbiol 44:2382-2388.
18. Mahony JB. 2008. Detection of respiratory viruses by molecular methods. Clin Microbiol Rev 21:716-747.
19. Babady NE, Mead P, Stiles J, Brennan C, Li H, Shuptar S, Stratton CW, Tang YW, Kamboj M. 2012. Comparison of the Luminex xTAG RVP Fast assay and the Idaho Technology FilmArray RP assay for detection of respiratory viruses in pediatric patients at a cancer hospital. J Clin Microbiol 50:2282-2288.
20. Webber DM, Wallace MA, Burnham CA, Anderson NW. 2020. Evaluation of the BioFire FilmArray Pneumonia Panel for Detection of Viral and Bacterial Pathogens in Lower Respiratory Tract Specimens in the Setting of a Tertiary Care Academic Medical Center. J Clin Microbiol 58.
21. Popowitch EB, O'Neill SS, Miller MB. 2013. Comparison of the Biofire FilmArray RP, Genmark eSensor RVP, Luminex xTAG RVPv1, and Luminex xTAG RVP fast multiplex assays for detection of respiratory viruses. J Clin Microbiol 51:1528-1533.
22. Ganzenmueller T, Kaiser R, Baier C, Wehrhane M, Hilfrich B, Witthuhn J, Flucht S, Heim A. 2020. Comparison of the performance of the Panther Fusion respiratory virus panel to R-Gene and laboratory developed tests for diagnostic and hygiene screening specimens from the upper and lower respiratory tract. J Med Microbiol 69:427-435.
23. Hologic I. 2020. Aptima SARS-CoV-2 (Panther System). Hologic, Inc.,10210 Genetic Center Drive, San Diego, CA 92121 USA, AW-21491-001 Rev. 001.
24. Cordes AK, Heim A. 2020. Rapid random access detection of the novel SARS-coronavirus-2 (SARS-CoV-2, previously 2019-nCoV) using an open access protocol for the Panther Fusion. J Clin Virol 125:104305.
25. Hologic I. 2020. SARS-CoV 2 Assay (Panther Fusion System). Hologic, Inc.,10210 Genetic Center Drive, San Diego, CA 92121 USA, AW-21159-001 Rev. 003.
26. Davis BM, Foxman B, Monto AS, Baric RS, Martin ET, Uzicanin A, Rainey JJ, Aiello AE. 2018. Human coronaviruses and other respiratory infections in young adults on a university campus: Prevalence, symptoms, and shedding. Influenza Other Respir Viruses 12:582-590.
27. Loens K, van Loon AM, Coenjaerts F, van Aarle Y, Goossens H, Wallace P, Claas EJ, Ieven M. 2012. Performance of different mono- and multiplex nucleic acid amplification tests on a multipathogen external quality assessment panel. J Clin Microbiol 50:977-987.
28. Gorzalski AJ, Tian H, Laverdure C, Morzunov S, Verma SC, VanHooser S, Pandori MW. 2020. High-Throughput Transcription-mediated amplification on the Hologic Panther is a highly sensitive method of detection for SARS-CoV-2. J Clin Virol 129:104501.
29. Pham J, Meyer S, Nguyen C, Williams A, Hunsicker M, McHardy I, Gendlina I, Goldstein DY, Fox AS, Hudson A, Darby P, Hovey P, Morales J, Mitchell J, Harrington K, Majlessi M, Moberly J, Shah A, Worlock A, Walcher M, Eaton B, Getman D, Clark C. 2020. Performance characteristics of a high throughput automated transcription mediated amplification test for SARS-CoV-2 detection. J Clin Microbiol doi:10.1128/jcm.01669-20.

medRxiv preprint doi: https://doi.org/10.1101/2020.08.31.20185074; this version posted September 2, 2020. The copyright holder for this preprint (which was not certified by peer review) is the author/funder, who has granted medRxiv a license to display the preprint in perpetuity.
It is made available under a CC-BY-NC-ND 4.0 International license .

30. Smith E, Zhen W, Manji R, Schron D, Duong S, Berry GJ. 2020. Analytical and Clinical Comparison of Three Nucleic Acid Amplification Tests for SARS-CoV-2 Detection. J Clin Microbiol doi:10.1128/jcm.01134-20.
31. Marando M, Tamburello A, Gianella P. 2020. False-Negative Nasopharyngeal Swab RT-PCR Assays in Typical COVID-19: Role of Ultra-low-dose Chest CT and Bronchoscopy in Diagnosis. Eur J Case Rep Intern Med 7:001680.
32. Ramos KJ, Kapnadak SG, Collins BF, Pottinger PS, Wall R, Mays JA, Perchetti GA, Jerome KR, Khot S, Limaye AP, Mathias PC, Greninger A. 2020. Detection of SARS-CoV-2 by bronchoscopy after negative nasopharyngeal testing: Stay vigilant for COVID-19. Respir Med Case Rep 30:101120.
33. Gualano G, Musso M, Mosti S, Mencarini P, Mastrobattista A, Pareo C, Zaccarelli M, Migliorisi P, Vittozzi P, Zumla A, Ippolito G, Palmieri F. 2020. Usefulness of bronchoalveolar lavage in the management of patients presenting with lung infiltrates and suspect COVID-19-associated pneumonia: A case report. Int J Infect Dis 97:174-176.
34. Hofmann H, Pyrc K, van der Hoek L, Geier M, Berkhout B, Pöhlmann S. 2005. Human coronavirus NL63 employs the severe acute respiratory syndrome coronavirus receptor for cellular entry. Proc Natl Acad Sci U S A 102:7988-7993.
35. Arden KE, Nissen MD, Sloots TP, Mackay IM. 2005. New human coronavirus, HCoV-NL63, associated with severe lower respiratory tract disease in Australia. J Med Virol 75:455-462.
36. Mateus J, Grifoni A, Tarke A, Sidney J, Ramirez SI, Dan JM, Burger ZC, Rawlings SA, Smith DM, Phillips E, Mallal S, Lammers M, Rubiro P, Quiambao L, Sutherland A, Yu ED, da Silva Antunes R, Greenbaum J, Frazier A, Markmann AJ, Premkumar L, de Silva A, Peters B, Crotty S, Sette A, Weiskopf D. 2020. Selective and cross-reactive SARS-CoV-2 T cell epitopes in unexposed humans. Science doi:10.1126/science.abd3871.
37. Pyrc K, Sims AC, Dijkman R, Jebbink M, Long C, Deming D, Donaldson E, Vabret A, Baric R, van der Hoek L, Pickles R. 2010. Culturing the unculturable: human coronavirus HKU1 infects, replicates, and produces progeny virions in human ciliated airway epithelial cell cultures. J Virol 84:11255-11263.

medRxiv preprint doi: https://doi.org/10.1101/2020.08.31.20185074; this version posted September 2, 2020. The copyright holder for this preprint (which was not certified by peer review) is the author/funder, who has granted medRxiv a license to display the preprint in perpetuity.
It is made available under a CC-BY-NC-ND 4.0 International license .

Table 1: Concentrations in PPR and final concentration in the PCR reaction. The concentration of the components in the PPR is higher by 1.25 x than in the final PCR reaction.

Substance	Concentration in PPR	Final concentration in PCR
MgCl	3.75 mM	3 mM
KCl	62.5 mM	50 mM
Tris buffer (pH8)	10 mM	8 mM
Primer for IC (fwd and rev)	0.94 µM	0.75 µM
Probe for IC	0.63 µM	0.5 µM
HCoV 229E N s (Primer)	0.5 µM	0.4 µM
HCoV 229E N as (Primer)	0.5 µM	0.4 µM
HCoV NL63 N s (Primer)	0.5 µM	0.4 µM
HCoV NL63 N as (Primer)	0.5 µM	0.4 µM
HCoV OC43 N s (Primer)	0.625 µM	0.5 µM
HCoV OC43 N as (Primer)	0.625 µM	0.5 µM
HCoV HKU1 N s (Primer)	0.625 µM	0.5 µM
HCoV HKU1 N as (Primer)	0.625 µM	0.5 µM
HCoV 229E (Probe)	0.25 µM	0.2 µM
HCoV NL63 (Probe)	0.25 µM	0.2 µM
HCoV OC43 (Probe)	0.625 µM	0.5 µM
HCoV HKU1 (Probe)	0.625 µM	0.5 µM

medRxiv preprint doi: https://doi.org/10.1101/2020.08.31.20185074; this version posted September 2, 2020. The copyright holder for this preprint (which was not certified by peer review) is the author/funder, who has granted medRxiv a license to display the preprint in perpetuity.
It is made available under a CC-BY-NC-ND 4.0 International license .

Table 2: Comparison of the PF LDT and the R-GENE CoV results

Diagnostic specimens (from URT and LRT)	**R-GENE positive**	**R-GENE negative**	**Total**
PF LDT positive	75	2	77
PF LDT negative	4	83	87
Total	79	85	164

medRxiv preprint doi: https://doi.org/10.1101/2020.08.31.20185074; this version posted September 2, 2020. The copyright holder for this preprint (which was not certified by peer review) is the author/funder, who has granted medRxiv a license to display the preprint in perpetuity.
It is made available under a CC-BY-NC-ND 4.0 International license .

Table 3: Comparison of three SARS-CoV-2 NATs to the consensus results.

Assay	**Consensus result**		**PPA**	**NPA**
	positive	**negative**		
Aptima SARS-CoV-2 TMA				
positive	56	1	100 %	99.0 %
negative	0	100		
LDT E-gene RT-PCR				
positive	56	1	100 %	99.0 %
negative	0	100		
Genesig COVID-19 RT-PCR				
positive	49	0	87.5 %	100 %
negative	7	101		
total	56	101		

medRxiv preprint doi: https://doi.org/10.1101/2020.08.31.20185074; this version posted September 2, 2020. The copyright holder for this preprint (which was not certified by peer review) is the author/funder, who has granted medRxiv a license to display the preprint in perpetuity.
It is made available under a CC-BY-NC-ND 4.0 International license .

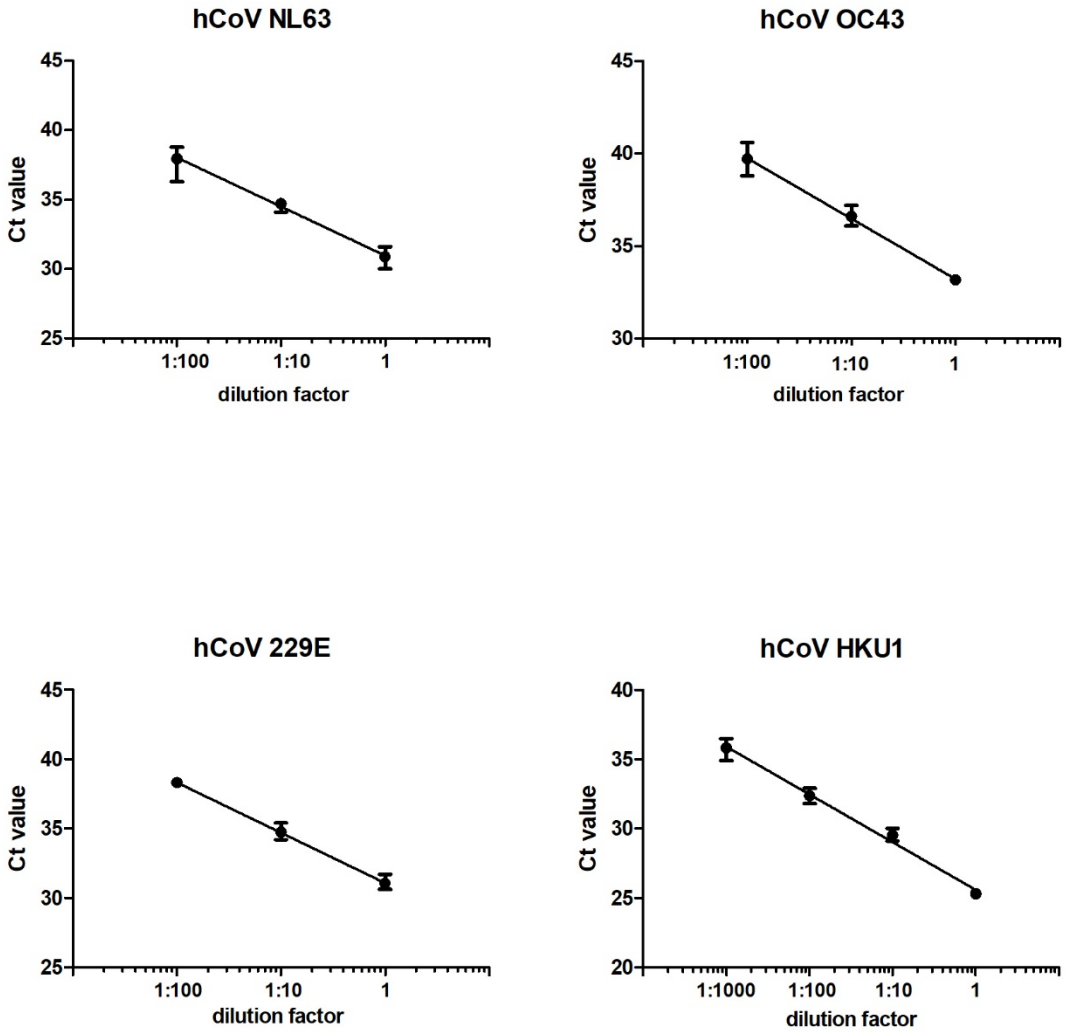

Figure 1: Amplification efficiency. For NL63, OC43 and 229E reference material from cell culture supernatants was applied. For the dilution series of HKU1, a highly positive diagnostic specimen was used. Each dot represents the mean out of three individual test results. The error bars display the range of Ct values.

Supplementary Table 1: Primer and probe sequences were used as published by Loens et al. Modifications were adapted for multiplexed use as shown in the table. All primers and probes were synthesized HPLC purified.

Name as in Loens et al. (27)	sequence	5' dye	3' quencher	internal quencher	company
HCoV 229E					
Primer 1	CAG TCA AAT GGG CTG ATG CA	-	-	-	Eurogentech
Primer 2	CAA AGG GCT ATA AAG AGA ATA AGG TAT TCT	-	-	-	Eurogentech
Probe A	CCC TGA CGA CCA CGT TGT GGT TCA	FAM	Iowa Black FQ	ZEN (after amino acid 9)	Integrated DNA Technologies
HCoV NL63					
Primer 3	GCG TGT TCC TAC CAG AGA GGA	-	-	-	Eurogentech
Primer 4	GCT GTG GAA AAC CTT TGG CA	-	-	-	Eurogentech
Probe B	ATG TTA TTC AGT GCT TTG GTC CTC GTG AT	HEX	Iowa Black FQ	ZEN (after amino acid 9)	Integrated DNA Technologies
HCoV OC43					
Primer 5	CGA TGA GGC TAT TCC GAC TAG GT	-	-	-	Eurogentech
Primer 6	CCT TCC TGA GCC TTC AAT ATA GTA ACC	-	-	-	Eurogentech
Probe C	TCC GCC TGG CAC GGT ACT CCC T	TYE665	Iowa Black RQ-Sp	-	Integrated DNA Technologies
HCoV HKU1					
864HCOV-HKU1s	TCC TAC TAY TCA AGA AGC TAT CC	-	-	-	Eurogentech
864HCOV-HKU1as	AAT GAA CGA TTA TTG GGT CCA C	-	-	-	Eurogentech
667HCOV-HKU1	TYC GCC TGG TAC GAT TTT GCC TCA	ROX (NHS Ester)	Iowa Black RQ-Sp	-	Integrated DNA Technologies

medRxiv preprint doi: https://doi.org/10.1101/2020.08.31.20185074; this version posted September 2, 2020. The copyright holder for this preprint (which was not certified by peer review) is the author/funder, who has granted medRxiv a license to display the preprint in perpetuity.
It is made available under a CC-BY-NC-ND 4.0 International license.

medRxiv preprint doi: https://doi.org/10.1101/2020.08.31.20185074; this version posted September 2, 2020. The copyright holder for this preprint (which was not certified by peer review) is the author/funder, who has granted medRxiv a license to display the preprint in perpetuity.
It is made available under a CC-BY-NC-ND 4.0 International license .

Supplementary table 2: Stability of the PPF on the PF. A PPR was pipetted and loaded onto the PF platform on day 0 and stayed on the platform for fourteen days. The same samples were tested on day 0, 6, 8 and 14.

	Sample	**material***	**Result Day 0 (Ct value)**	**Result Day 6 (Ct value)**	**Result Day 8 (Ct value)**	**Result Day 14 (Ct value)**
1	NC**	BL	negative	negative	negative	negative
2	NC**	NPS	negative	negative	negative	negative
3	229E	NPS	25.5	26.3	26.0	26.4
4	229E	PL	34.4	34.4	33.3	33.9
5	NL63	PL	19.2	18.0	18.8	19.3
6	NL63	BAL	34.4	34.1	34.2	35.0
7	HKU1	BAL	26.9	25.7	27.2	28.7
8	HKU1	BAL	36.6	38.1	36.5	37.5
9	OC43	NPS	23.9	24.3	26.3	24.5
10	OC43	BAL	36.9	39.4	38.7	38.0

* bronchial alveolar lavages (BAL), bronchial lavages (BL), nasal swabs (NS), nasopharyngeal swabs (NPS), pharyngeal lavages (PL), tracheal swabs (TRS), tracheal secretions (TS)

** negative control (NC)

medRxiv preprint doi: https://doi.org/10.1101/2020.08.31.20185074; this version posted September 2, 2020. The copyright holder for this preprint (which was not certified by peer review) is the author/funder, who has granted medRxiv a license to display the preprint in perpetuity.
It is made available under a CC-BY-NC-ND 4.0 International license .

Supplementary table 3: Those samples that were found to be positive in at least two out of three assays were declared as consensus positive. For negative samples the criteria was implemented respectively.

Material*	**Aptima SARS-CoV-2**		**E-gene LDT RT-PCR**		**Genesig RT-PCR**	
	positive of consensus positive	negative of consensus negative	positive of consensus positive	negative of consensus negative	positive of consensus positive	negative of consensus negative
BAL	5/5	3/3	5/5	3/3	4/5	3/3
BL	5/5	2/2	5/5	2/2	4/5	2/3
NS	3/3	3/3	3/3	3/3	3/3	3/3
NPS	38/38	86/87	38/38	86/87	34/38	87/87
PL	0/0	1/1	0/0	1/1	0/0	1/1
TRS	3/3	4/4	3/3	4/4	2/3	4/4
TS	2/2	1/1	2/2	1/1	2/2	1/1

*bronchial alveolar lavages (BAL), bronchial lavages (BL), nasal swabs (NS), nasopharyngeal swabs (NPS), pharyngeal lavages (PL), tracheal swabs (TRS), tracheal secretions (TS)