medRxiv preprint doi: https://doi.org/10.1101/2021.01.13.21249563; this version posted January 15, 2021. The copyright holder for this preprint (which was not certified by peer review) is the author/funder, who has granted medRxiv a license to display the preprint in perpetuity. All rights reserved. No reuse allowed without permission.

COVID-19: Rapid Antigen detection for SARS-CoV-2 by lateral flow assay: a national systematic evaluation for mass-testing

UK COVID-19 Lateral Flow Oversight Team

Corresponding Author:

Prof Tim Peto

Senior Author: Professor Tim Peto, Nuffield Department of Medicine, University of Oxford

Running Title: Clinical utility of lateral flow SARS-CoV-2 antigen detection

Keywords: coronavirus, COVID-19, SARS-CoV-2, United Kingdom, Public Health, lateral flow, viral antigen detection, testing, national evaluation, LFD, lateral flow tests, lateral flow devices.

NOTE: This preprint reports new research that has not been certified by peer review and should not be used to guide clinical practice.

medRxiv preprint doi: https://doi.org/10.1101/2021.01.13.21249563; this version posted January 15, 2021. The copyright holder for this preprint (which was not certified by peer review) is the author/funder, who has granted medRxiv a license to display the preprint in perpetuity. All rights reserved. No reuse allowed without permission.

Abstract

Background: New lateral flow device (LFD) viral antigen immunoassays have been developed by commercial and research organisations around the world as diagnostic tests for SARS-CoV-2 infection. To support decisions by the UK Government on potential scale-up of mass population testing, we have at their request evaluated the diagnostic performance of a significant number of point-of-care rapid SARS-CoV-2 LFDs.

Methods: 132 LFDs were initially reviewed by a Department of Health and Social Care team, part of the UK government, from which 64 were selected for further evaluation. Standardised laboratory evaluations, and for those that met the published criteria, field testing in the Falcon-C19 research study and UK pilots were performed (UK COVID-19 testing centres, hospital, schools, armed forces).

Results: 4/64 LFDs so far have desirable performance characteristics from independent laboratory studies and early preliminary field evaluations (Orient Gene, Deepblue and *Innova SARS-CoV-2 Antigen Rapid Qualitative Test*), of which one underwent extended clinical assessment in field studies (*Innova*). 8951 Innova LFD tests were performed with a kit failure rate of 5.6% (502/8951, 95% CI: 5.1-6.1), false positive rate of 0.32% (22/6954, 95% CI: 0.20-0.48) and a viral antigen detection/sensitivity (using RNA RT-PCR as a proxy for the presence of antigen) of 78.8% when performed by laboratory scientists (156/198, 95% CI 72.4-84.3). Sensitivity was significantly lower when testing was undertaken by non-experts with limited initial training

Interpretation: Several LFDs have promising performance characteristics for mass population testing and can be used to identify infectious positive individuals. The Innova LFD shows good viral antigen detection/sensitivity with excellent specificity, although kit failure rates and the impact of training are potential issues. These results support the expanded evaluation of LFDs, and assessment of greater access to testing on COVID-19 transmission.

Funding: Department of Health and Social Care. University of Oxford. Public Health England Porton Down, Manchester University NHS Foundation Trust, National Institute of Health Research.

medRxiv preprint doi: https://doi.org/10.1101/2021.01.13.21249563; this version posted January 15, 2021. The copyright holder for this preprint (which was not certified by peer review) is the author/funder, who has granted medRxiv a license to display the preprint in perpetuity. All rights reserved. No reuse allowed without permission.

Introduction

National governments and international organisations including the World Health Organisation (WHO) and European Commission have highlighted the importance of individual testing, mass population testing and subsequent contact tracing to halt the chain of transmission of SARS-CoV-2, the virus responsible for COVID-19.[1,2,3] The current diagnostic test involves reverse-transcription polymerase chain reaction (RT-PCR) testing of nose/throat swabs in specialised laboratories. Such capacity in the UK is currently estimated at ~500,000 tests/day[4–7] and this is used with contact tracing procedures and mobile applications to identify close symptomatic contacts of infected symptomatic individuals.[8–10] However, there are significant challenges in creating testing capacity to identify those with asymptomatic infections or to test contacts of individuals with COVID-19. To date, turnaround time for RT-PCR has been typically slow (>24 hours).

To better understand and control SARS-CoV-2 transmission, there is an urgent need for large-scale, accurate, affordable and rapid diagnostic testing assays, with the ability to detect infectious individuals. Lateral flow device (LFD) immunoassays can be designed to test for different protein targets and are routinely used in healthcare settings principally as a result of their affordability, ease of use, short turnaround time, and high-test accuracy. In brief, a sample is placed on a conjugation pad where the analyte (or antigen) of interest is bound by conjugated antibodies. The analyte-antibody mix subsequently migrates along a membrane by capillary flow across both 'test' and 'control' strips. These strips are coated with antibodies detecting the analyte of interest and a positive test is confirmed by the appearance of coloured control and test lines.[11]

Newly developed SARS-CoV-2 antigen LFDs identify the presence of specific viral proteins, using conjugated antibodies to bind spike, envelope, membrane or nucleocapsid proteins. In contrast to the IgM/IgG "antibody tests", these antigen tests directly identify viral proteins, and are not reliant on the host's immune response. In contrast to RT-PCR, results for LFDs are observed in 10-30 minutes depending on the device, providing a window for early interventions to halt the chain of transmission earlier in the disease course when individuals are most infectious.[12]

To date, many manufacturers have developed first-generation rapid SARS-CoV-2 antigen-detecting LFDs. However, many of these tests have not been independently validated. There is evidence of variable performance when assessing test sensitivity and specificity, although several candidates looked promising on the basis of early data.[13–15] An independent national evaluation of these devices is important to facilitate population-level or mass testing initiatives globally.

Here, we report the diagnostic performance of first-generation SARS-CoV-2 antigen-detecting LFD for rapid point-of-care (POC) testing in work that was commissioned by the UK's Department of Health and Social Care (DHSC) from PHE Porton Down and the University of Oxford.

medRxiv preprint doi: https://doi.org/10.1101/2021.01.13.21249563; this version posted January 15, 2021. The copyright holder for this preprint (which was not certified by peer review) is the author/funder, who has granted medRxiv a license to display the preprint in perpetuity. All rights reserved. No reuse allowed without permission.

Methods

A phased evaluation of available SARS-CoV-2 antigen LFDs was undertaken.

Department of Health and Social Care evaluation (Phase 1 evaluation)

The DHSC identified manufacturers supplying SARS-CoV-2 antigen LFDs that could enable mass testing at a population level. A desktop review was performed to ensure there were appropriate instructions for use and to assess manufacturers' claimed performance and manufacturing capabilities.[16]

Pre-clinical evaluation (Phase 2 evaluation)

Pre-clinical evaluation of candidate LFDs was performed by trained laboratory scientists at Public Health England (PHE) Porton Down. LFDs were evaluated against SARS-CoV-2 spiked positive controls and known negative controls, consisting of saliva collected from healthy adult staff volunteers.

Pre-defined and publically available "prioritisation" criteria to pass on to the next evaluation phase had to be met for LFDs, consisting of (i) a kit failure rate of <10%; (ii) an analytical specificity of ≥97%, and (iii) an analytical LOD of $\geq$9 of 15 (60%) at 10^2 pfu/mL, corresponding to a RT-PCR cycle threshold (Ct) of approximately 25 (~100,000 RNA copies/ml); and (iv) lack of cross-reactivity with seasonal coronaviruses to further test analytical specificity.

Retrospective secondary care evaluation (Phase 3a evaluation)

Evaluation using patient samples retrospectively was started in August 2020 at PHE Porton Down. Samples were obtained from a secondary healthcare setting (Oxford University Hospitals NHS Foundation Trust).

- 1,000 SARS-CoV-2 negative samples: fresh samples held refrigerated were supplied the day after they were tested negative by RT-PCR by the laboratory service at the John Radcliffe Hospital, Oxford, UK.
- 200 SARS-CoV-2 positive samples: swabs collected in VTM from patients admitted to hospital during the first wave of the UK pandemic (March-June 2020).[17] These were diluted 1:4 SARS-CoV-2 RT-PCR negative saliva, aliquoted and frozen at -20°C for later use. For each positive sample, in addition to the original diagnostic RT-PCR Ct value, a confirmatory RT-PCR was performed at PHE Porton Down on the diluted sample to determine the new Ct value.

Community research evaluation (Phase 3b evaluation)

We undertook a field evaluation using samples from volunteers in the community in collaboration with the National Institute for Health Research (NIHR) funded CONDOR Platform "COVID-19 National Diagnostic Research and Evaluation Platform". This was performed within the FALCON-C19 study (Facilitating Accelerated Clinical validation Of Novel diagnostics for COVID-19, 20/WA/0169, IRAS 284229), between 17th September and 23rd October 2020. This involved the recruitment and re-testing of consenting adults with a RT-PCR-confirmed diagnosis of SARS-CoV-2 infection within 5 days of the original PCR result.

For the *Innova SARS-CoV-2 Antigen Rapid Qualitative Test*, testing was additionally performed for a subset of samples on-site at four COVID-19 testing centres by trained research staff using the "dry swabs" to evaluate "real-life"/diagnostic performance. Dry swabs are those that are not placed into viral transport medium prior to performing the LFD test.

Community field service evaluation (Phase 4 evaluation)

Wider field service evaluations were performed within a number of UK institutions and settings. These evaluations utilised the *Innova SARS-CoV-2 Antigen Rapid Qualitative Test*. These institutions included a secondary healthcare setting (John Radcliffe Hospital, Oxford), PHE Porton Down, armed forces members (following an outbreak) and in secondary schools (pupils aged 11-18). Evaluations were also undertaken at regional COVID-19 testing centres as part of an NHS Test and Trace service evaluation involving the general public. The John Radcliffe Hospital, Oxford performed an evaluation as part of their asymptomatic staff screening service using the Respiratory Diagnostic Kit Evaluation ('Red Kite') study (Research Ethics Committee reference: 19/NW/0730; North West-Greater Manchester South Research Ethics Committee).

Statistical analyses

Fisher's exact and chi-squared tests were used to determine non-random associations between categorical variables. Statistical analyses and data visualisation were performed using R version 4.0.3. Sensitivity and specificity and 95% confidence intervals were calculated using the exact Clopper-Pearson method.

medRxiv preprint doi: https://doi.org/10.1101/2021.01.13.21249563; this version posted January 15, 2021. The copyright holder for this preprint (which was not certified by peer review) is the author/funder, who has granted medRxiv a license to display the preprint in perpetuity. All rights reserved. No reuse allowed without permission.

Results

Phase 1

A total of 132 suppliers of SARS-CoV-2 antigen detection LFDs were identified and referred to the DHSC for initial Phase 1 review. Among these, at the time of publication, 64 were selected by the DHSC for further evaluation by the UK lateral flow oversight group.

Phase 2

As part of Phase 2 evaluations, 9,692 LFD tests were performed at PHE Porton Down across the 64 candidate devices as of the 3rd December 2020. 5 LFDs had a kit failure rate above the pre-specified threshold for exclusion (>10%), 17 kits had a false-positive rate below the pre-defined specificity threshold (<97%) and 28 kits a false-negative rate below the LOD threshold (<60% at 10^2 pfu/m). In total, across all three criteria, nineteen kits performed at a level in accordance with the UK Lateral Flow Oversight Group's *a priori* "prioritisation criteria". All nineteen kits also passed cross-reactivity analyses against seasonal human coronaviruses.

Phase 3

To date, eight LFDs have passed Phase 3a evaluation, namely: *Innova SARS-CoV-2 Antigen Rapid Qualitative Test* (Innova)*, Zhejiang Orient Gene Biotech Co. Coronavirus Ag Rapid Test Cassette* (Swab) (Orient Gene)*, Anhui Deepblue Medical Technology COVID-19 (Sars-CoV-2) Antigen Test kit (Colloidal Gold) (*Deepblue)*, Fortress Diagnostics Coronavirus Ag Rapid Test (Fortress), Roche SD Biosensor Standard Q COVID-19 Ag Test (SD Bio swab), Surescreen Diagnostics SARS-CoV-2 Antigen Rapid Test Cassette (Nasopharyngeal swab (Surescreen) and LFD x (the manufacturer had not given consent to be named).* (Supplementary Table 1). Three LFDs did not pass 3a evaluation and the remaining LFDs are currently undergoing evaluation. Four LFDs (Deepblue, Innova, Orientgene, LFD x) have passed Phase 3b evaluation (Table 1, Supp Figure 1), one LFD did not pass and the remainder have not been evaluated.

Viral Load	Average Ct	Innova Number tested/number positive (%)	LFD x Number tested/number positive (%)	Orient Gene Number tested/number positive (%)	Deepblue Number tested/number positive (%)
>10million	<18	5/5 (100)	1/1 (100)	-	3/3 (100)
1-10 million	18-21.5	23/23 (100)	12/13 (92)	17/17 (100)	19/19 (100)
0.1-1 million	21.5-25	52/54 (96)	19/21 (91)	18/18 (100)	43/44 (98)
10,000-100,000	25-28	37/42 (88)	13/13 (100)	18/19 (95)	38/38 (100)
1,000-10,000	28-31	25/33 (76)	17/19 (90)	14/18 (78)	18/29 (62)
100-1,000	31-34.5	11/33 (33)	10/26 (39)	11/19 (58)	8/36 (22)
<100	>34.5	2/7 (29)	1/6 (17)	0/4 (0)	0/8 (0)
Overall	na	155/197 (79)	73/99 (74)	78/95 (82)	129/177(73)

Table 1. Results of the Phase 3b evaluations showing viral antigen detection/sensitivity of four LFD tests using dry-swab samples from community sampling. Tests were performed by laboratory scientists. Ct – cycle threshold on RT-PCR.

Extended Innova LFD evaluation (Phases 2-4)

The limit of detection of the Innova LFD (Table 2) was determined as part of Phase 2 evaluations for the Innova test. This analysis consisted of saliva spiked with SARS-CoV-2 with stock of SARS-CoV-2 with a standardised PFU. Under these ideal concentrations, at an estimated PFU of 390/mL, which corresponds to a Ct of ~25, the LFD identified all samples.

PFU/ml	Ct equivalent	Positive LFD tests/total LFD tests	% positive
100000	16	20/20	100
10000	19	25/25	100
1000	23.7	65/65	100
390	25.2	5/5	100
100	25.5	63/65	96
40	28.5	3/5	60
20	29.3	0/5	0
10	30.2	0/5	0
5	31	0/5	0
2.5	31.7	0/5	0
1.2	32.5	0/5	0

Table 2. Limit of sensitivity for SARS-CoV-2 detection by the Innova LFD for antigen detection using saliva sample spiked with SARS-CoV-2. Ct - cycle threshold. PFU - plaque forming units.

medRxiv preprint doi: https://doi.org/10.1101/2021.01.13.21249563; this version posted January 15, 2021. The copyright holder for this preprint (which was not certified by peer review) is the author/funder, who has granted medRxiv a license to display the preprint in perpetuity. All rights reserved. No reuse allowed without permission.

Our phase 4 evaluation focused on field testing of the Innova LFD, for which we had a sufficient supply of kits available for wider testing at the time. Device specificity was determined through an analysis of 6954 tests from evaluation phases 2-4. The percentage of false-positives ranged from 0.00-0.49%, with an overall specificity of 99.68%. The false-positive rate was centre-dependent (p=0.014, Fisher's exact test). These evaluations noted that where there were challenges in interpreting the results when the test result was "weak" (i.e. the test line was very faint) (Table 3).

Evaluation Phase	False positives/total number	False positives and 95% confidence interval
Phase 2 evaluation	0/72	0.0% (0.0-5.0)
Phase 3a evaluation- negative samples	0/940	0.0% (0.0-0.4)
Phase 4 evaluation- hospital staff	1/329*	0.3% (0.01-1.7)
Phase 4 evaluation- armed forces	0/105	0.0% (0.0-3.5)
Phase 4 evaluation- PHE staff	0/209	0.0% (0.0-1.8)
Phase 4 evaluation- school 1	9/1855**	0.5% (0.2-0.9)
Phase 4 evaluation- school 2 + 3 + 4	7/2130**	0.3% (0.1-0.7)
Phase 4 evaluation- COVID-19 testing centre	5/1314***	0.4% (0.1-0.9)
TOTAL	22/6954	0.3% (0.2-0.5)

*This was 1 weak positive result that was also a weak positive on repeating; ** Weak positives result were negative on retesting with Innova; *** Not photographed or repeated. Taken in a setting of prevalence of 14% LFD positive results.

Table 3. Number of false positives in negative samples in each evaluation stage for the Innova LFD. 95% confidence intervals presented in each case.

Across Phase 2-4 evaluation stages, 8,951 Innova LFD tests were performed, including a diverse cohort of populations as part of Phase 3b and Phase 4 testing, namely out-patient SARS-CoV-2 cases, healthcare staff, armed forces personnel and secondary school children. The overall kit failure rate for the Innova LFD was 5.6% (502/8951, 95% CI: 5.1-6.1) (Table 4). The most common reason for kit failure was poor transfer of the liquid within the device from the reservoir onto the test strip.

Innova LFD evaluation phase	LFD failures (%)
Phase 2 negatives	0/72 (0.0%)
Phase 2 positive dilution series	0/60 (0.0%)
Phase 2 positive extended dilution series	0/155 (0.0%)
Phase 2 Swab comparison	0/187 (0.0%)
Phase 3a positives	13/191 (6.8%)
Phase 3a negatives	50/990 (5.1%)
Phase 3b FALCON (Dry swabs- field)	27/267 (10.1%)
Phase 3b FALCON (Dry swabs- lab)	9/212 (4.2%)
Phase 3b FALCON (VTM swabs)	9/157 (5.7%)
Phase 4 hospital staff	17/358 (4.7%)
Phase 4 armed forces	6/157 (3.8%)
Phase 4 PHE staff	19/212 (8.9%)
Phase 4 school 1	311/1855 (16.8%)
Phase 4 school 2 + 3 + 4	14/2132 (0.7%)
Phase 4 COVID-19 testing centre	27/1946 (1.4%)
	502/8951 (5.6%)

Table 4. Evaluations of the Innova LFD across Phases 2-4. The table demonstrates the kit failure rate.

Viral antigen detection/sensitivity in individuals with confirmed SARS-CoV-2 infection using the Innova LFD was assessed in the Phase 3b evaluation as part of the FALCON-C19 research study. Optimal viral antigen detection/sensitivity when performed by laboratory scientists, was 78.8% (95% CI 72.4-84.3%; 156/198 cases where a paired PCR was performed; see below for differing performance by test operator category). Subgroup analyses showed there were no discernible differences in viral antigen detection/sensitivity in those without symptoms vs. symptomatic individuals (27/41 [65.9%] vs. 95/344 [72.4%], p=0.38). We did not find any evidence of associations between LFD positivity and symptoms or past medical history, with the exception of presence of headache (Supplementary Table 2).

The association between Innova LFD viral antigen detection/sensitivity and estimated viral load/Ct value was explored using the paired RT-PCR VTM swab sample taken at the same time as the swab used for LFD. There was a strong association between viral load detection (RNA copies/mL) determined through RT-PCR and viral antigen detection by LFD (Figure 1). Confirming earlier analyses, sensitivity of LFDs is highest in samples with higher viral loads.[18 19]

medRxiv preprint doi: https://doi.org/10.1101/2021.01.13.21249563; this version posted January 15, 2021. The copyright holder for this preprint (which was not certified by peer review) is the author/funder, who has granted medRxiv a license to display the preprint in perpetuity. All rights reserved. No reuse allowed without permission.

Within the 3b FALCON-C19 study, LFDs were also assessed by sampling 150uL of viral transport medium (VTM) solution instead of using dry swabs; this was associated with poorer performance rate (Supp Figure 2). The use of dry swabs forms the basis of the manufacturer's instructions for use. This was likely due to a dilution factor involved in placing the swab first into VTM and then analysing the VTM sample, and highlights potential issues in generating direct comparisons between LFDs and VTM samples (Supp Figure 2).

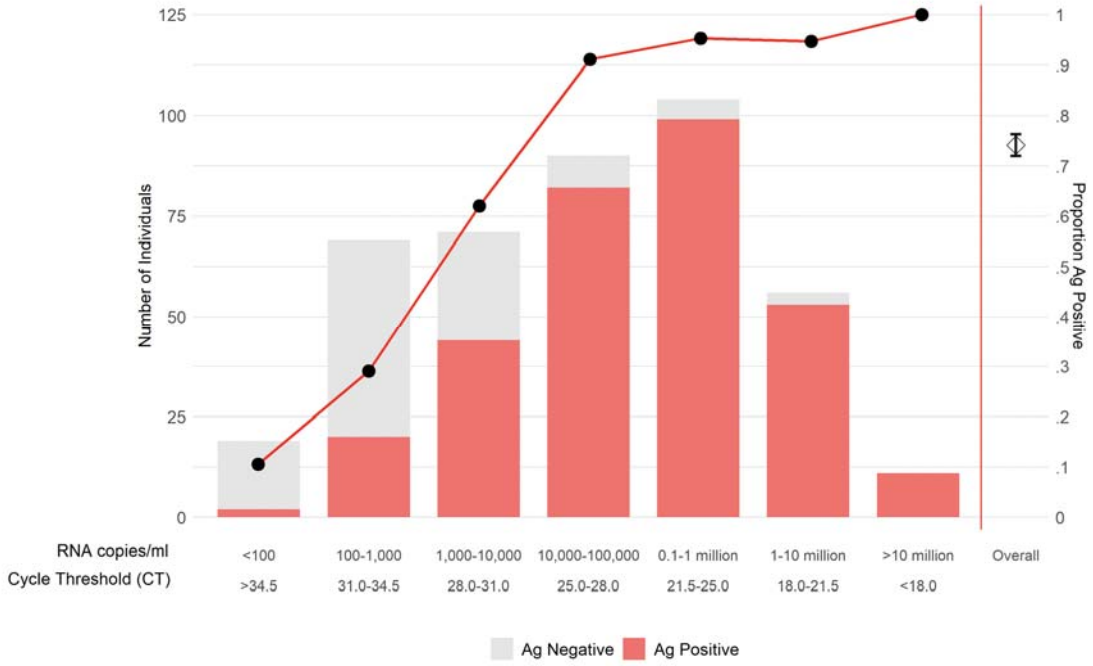

Figure 1. Association between viral antigen detection/sensitivity and viral load (RNA copies/mL and Ct) in Phase 3b Falcon-C19 study evaluation for dry swabs when performed by trained laboratory scientists and trained healthcare workers. Diamond shows point estimate, with 95% confidence intervals, pooling data from all other categories.

As part of Phase 3b-4 evaluations, work was performed to report on the effect of the operator on viral antigen detection/sensitivity in RT-PCR-positive cases using the Innova LFD. Tests were classified according to whether they were performed by a laboratory scientist, a fully trained research health care worker or by a self-trained lay individual working at a regional NHS Test and Trace centre. Performance was optimal when the LFD was used by laboratory scientists (156/198 LFDs positive [78.8%, 95% CI: 72.4-84.3%]) relative to trained healthcare-workers (156/223 LFDs positive [70.0%, 95% CI: 63.5-75.9%]) and self-trained members of the public given a protocol (214/372 LFDs positive [57.5%, 95% CI: 52.3-62.6%]; p<0.0001).

medRxiv preprint doi: https://doi.org/10.1101/2021.01.13.21249563; this version posted January 15, 2021. The copyright holder for this preprint (which was not certified by peer review) is the author/funder, who has granted medRxiv a license to display the preprint in perpetuity. All rights reserved. No reuse allowed without permission.

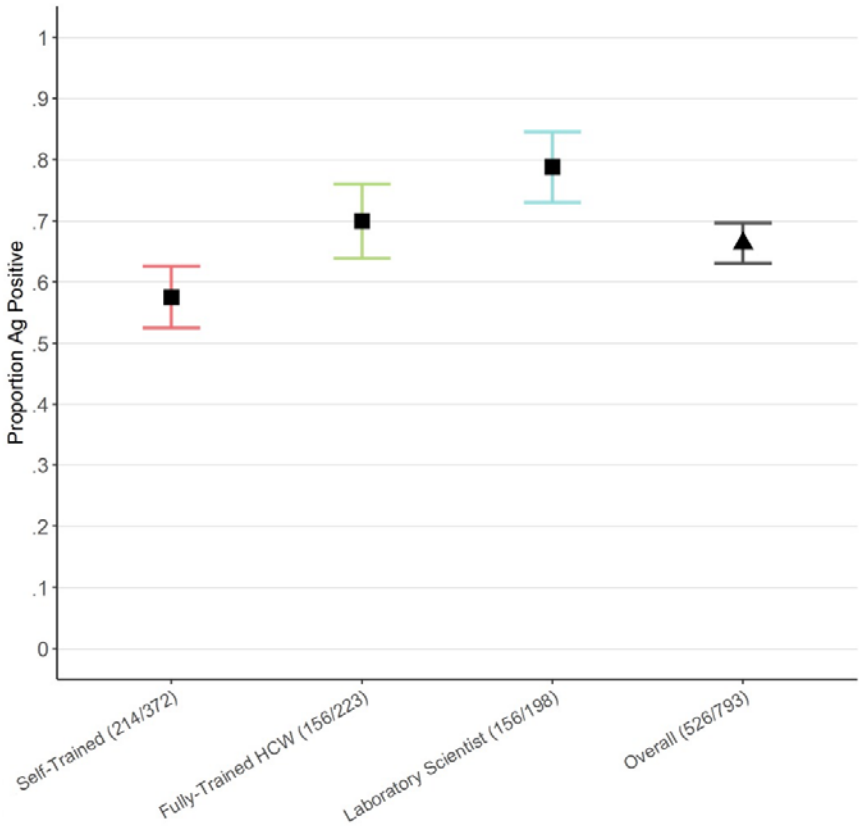

Figure 2. Effect of training and operator on the viral detection/sensitivity of the Innova LFD in COVID-19 PCR-positive patients.

medRxiv preprint doi: https://doi.org/10.1101/2021.01.13.21249563; this version posted January 15, 2021. The copyright holder for this preprint (which was not certified by peer review) is the author/funder, who has granted medRxiv a license to display the preprint in perpetuity. All rights reserved. No reuse allowed without permission.

Discussion

We report on our national evaluation of SARS-CoV-2 viral antigen-detecting LFDs, focussing on the *Innova SARS-CoV-2 Antigen Rapid Qualitative Test,* which has a viral antigen detection (sensitivity) of 78.8% when performed by laboratory scientists and a specificity of 99.7%, using RT-PCR as 'gold standard' for positive and negative status. In our evaluation, test performance was largely maintained across different settings and cohorts; however, performance was partly operator-dependent and kit failures are not infrequent.

Test performance to detect SARS-CoV-2-positive samples was improved at lower Ct values/higher viral loads, and were >90% at Ct values <25 equating to ~390 pfu/mL (Supplementary Table 3). There is an expanding body of evidence that suggests viral load/antigen is important as individuals with the highest viral loads are the most infectious, [20] and the presence/absence of viral antigens determined by LFDs is more strongly associated with a viral culture than RT-PCR positivity.[21]

Our experience is that many LFDs entering our national evaluation program do not perform at a level required for mass population deployment and this reflects the literature. To date, an increasing number of evaluations of SARS-CoV-2 antigen-detecting LFD have been published with variable results. A number of LFDs show good[24] [25] [13] [19] [26] [27] or acceptable sensitivity and specificity[28] [29], however, many studies have identified tests with poor sensitivities or specificities.[30] [15]

A challenge for most countries during the SARS-CoV-2 pandemic has been the expansion of capacity for diagnostic testing to support the identification of symptomatic and asymptomatic cases. This would aid in offering testing to "contacts" of COVID-19 and enable targeted testing to better safeguard vulnerable populations e.g. care home residents. Reliance on RT-PCR involves significant infrastructural and specialist human resources to implement at increasing scale. Both the World Health Organisation and European commission have issued guidance supporting wider implementation of antigen-targeting LFDs, and in November, Slovakia became the first country in the world to implement entire population testing using LFDs. [1,3,31] The UK has similar aspirations to pursue a strategy of mass testing and has implemented a city wide mass testing in Liverpool using the Innova LFD in this study.[32]

It is important to note that there are some potential issues with considering RT-PCR as the gold standard test for COVID-19. Many individuals have persisting viral RNA fragments that can linger for weeks-months without any evidence of active viral replication; in this instance a PCR-positive is likely to overcall the "infectious" status of an individual [33] Indeed, when compared to the ability to perform viral culture, data suggest that RT-PCR tends to overestimate the presence of replicating or infectious virions.[34]

In field testing, performance of the Innova LFD was dependent on the test operator. Individuals who had read a protocol immediately prior to self-sampling did not perform as well as individuals with hands-on training, or clinical laboratory personnel who had performed several hundred LFD tests. Like other operator-dependent procedures, further work is required to determine the duration and content of "training" to derive optimal test performance. We also assume that the use of LFDs to successfully identify individuals with higher viral loads and enabling an earlier diagnosis will be of benefit in interrupting transmission, however, this remains to be proven.

SARS-CoV-2 control will benefit from a variety of testing strategies. This might include those optimised for determining past infection/exposure (e.g. serology), those that are of benefit in determining current/recent infection (e.g. RT-PCR), or those identifying potential infectivity. A combination of approaches incorporating the strengths of each of these tests can be effectively used for individuals and for population-level management of the pandemic. Approaches to testing will remain relevant even when effective vaccines become available as it may take several months for an appreciable effect on transmission to be fully realised.[35]

In conclusion, we completed late stage evaluations of seven LFDs. We report sensitivities of 70-80% and specificities ≥99.7% for each LFD evaluated in phase 3b, which involved testing by laboratory personnel or trained healthcare professionals. To identify patients with higher viral loads (Ct<25), each LFD had >90% sensitivity. Sensitivity was lower in phase 4 evaluations, while specificity was maintained. The simplicity of LFDs, without a requirement for specialist training or equipment, mean that they are an attractive option for mass testing. Future research should focus on post-implementation evaluation of diagnostic accuracy, including the potential benefit of regular serial sampling to improve accuracy and reduce transmission.

medRxiv preprint doi: https://doi.org/10.1101/2021.01.13.21249563; this version posted January 15, 2021. The copyright holder for this preprint (which was not certified by peer review) is the author/funder, who has granted medRxiv a license to display the preprint in perpetuity. All rights reserved. No reuse allowed without permission.

Acknowledgements

The authors thank the participants and their families affected by COVID-19, NHS doctors and nurses and other medical staff, research scientists and support staff at Public Health England, Porton Down, NHS Test and Trace COVID-19 testing centres staff, the NIHR research network, the University of Birmingham medical school, the University of Oxford medical school, the University of Newcastle medical school, NHS Test and Trace and St John Ambulance.

We would like to thank all members of the UK Lateral flow oversight group in contributing data at a challenging time as listed in the web appendix (appendix page 1)

We would like to acknowledge the Department of Health and Social Care, NIHR, University of Manchester and University of Oxford Biomedical Research Council in funding this study.

Viral stocks were supplied by Dr Julian Druce, Doherty Institute, Queensland University, Australia.

The NHS and funders had no role in data collection, analysis or decision to publish.

Funding statement

DSL is supported by the NIHR Community Healthcare MedTech and In vitro Diagnostic Cooperative and the NIHR Applied Research Collaboration (ARC) West Midlands. LYWL, DWC, TEAP, AV, SJH, ASW and HLP are supported by the NIHR Oxford BRC. DWC and NS are supported by the National Institute for Health Research (NIHR) Health Protection Research Unit in Healthcare Associated Infections at University of Oxford (NIHR200915) in partnership with Public Health England (PHE). KKC is Medical Research Foundation-funded. DWC, ASW and TEAP are NIHR Senior Investigators. PCM is funded by the Wellcome Trust (grant 110110/Z/15/Z). Falcon-C19 is a project funded by a National Institute for Health Research (NIHR). DWE is a Robertson Foundation Big Data Institute Fellow. SFL is funded by a Wellcome Trust Clinical Research Fellowship.

The report presents independent research funded by the National Institute for Health Research, Wellcome Trust and the Department of Health. The views expressed in this publication are those of the authors and not necessarily those of the NHS, Wellcome Trust, the National Institute for Health Research, the Department of Health or Public Health England.

Declaration of interest

DWE declares lecture fees from Gilead, outside the submitted work. LYWL has previously received speaker honorarium from the Merck group and Servier for unrelated work. The other authors have nothing to disclose.

medRxiv preprint doi: https://doi.org/10.1101/2021.01.13.21249563; this version posted January 15, 2021. The copyright holder for this preprint (which was not certified by peer review) is the author/funder, who has granted medRxiv a license to display the preprint in perpetuity. All rights reserved. No reuse allowed without permission.

References

1. Diagnostic testing for SARS-CoV-2. https://www.who.int/publications/i/item/diagnostic-testing-for-sars-cov-2.
2. Raffle, A. E., Pollock, A. M. & Harding-Edgar, L. Covid-19 mass testing programmes. *The BMJ* vol. 370 (2020).
3. Commission steps up actions on testing. *European Commission - European Commission* https://ec.europa.eu/commission/presscorner/detail/en/ip_20_2047.
4. How is the COVID-19 Virus Detected using Real Time RT-PCR? | IAEA. https://www.iaea.org/newscenter/news/how-is-the-covid-19-virus-detected-using-real-time-rt-pcr.
5. EMERGENCY USE AUTHORIZATION (EUA) SUMMARY COVID-19 RT-PCR TEST (LABORATORY CORPORATION OF AMERICA). https://www.fda.gov/media/136151/download.
6. Ghoshal, U., Vasanth, S. & Tejan, N. A guide to laboratory diagnosis of Corona Virus Disease-19 for the gastroenterologists. *Indian Journal of Gastroenterology* vol. 39 236–242 (2020).
7. Coronavirus (COVID-19) in the UK: Testing. https://coronavirus.data.gov.uk/testing.
8. NHS Test and Trace: how it works - GOV.UK. https://www.gov.uk/guidance/nhs-test-and-trace-how-it-works.
9. NHS COVID-19 - NHS. https://www.nhs.uk/apps-library/nhs-covid-19/.
10. Coronavirus (COVID-19): Contact tracing in Scotland | NHS inform. https://www.nhsinform.scot/illnesses-and-conditions/infections-and-poisoning/coronavirus-covid-19/test-and-protect/coronavirus-covid-19-contact-tracing.
11. O'Farrell, B. Evolution in Lateral Flow–Based Immunoassay Systems. in *Lateral Flow Immunoassay* 1–33 (Humana Press, 2009). doi:10.1007/978-1-59745-240-3_1.
12. Guglielmi, G. Fast coronavirus tests: what they can and can't do. *Nature* **585**, 496–498 (2020).
13. Porte, L. *et al.* Evaluation of a novel antigen-based rapid detection test for the diagnosis of SARS-CoV-2 in respiratory samples. *Int. J. Infect. Dis.* **99**, 328–333 (2020).
14. Mertens, P. *et al.* Development and Potential Usefulness of the COVID-19 Ag Respi-Strip Diagnostic Assay in a Pandemic Context. *Front. Med.* **7**, 225 (2020).
15. Denkinger, C. Evaluation of the accuracy, ease of use and limit of detection of novel, rapid, antigen-detecting point-of-care diagnostics for SARS-CoV-2. *medRxiv* 2020.10.01.20203836 (2020) doi:10.1101/2020.10.01.20203836.
16. Protocol for evaluation of rapid diagnostic assays for specific SARS-CoV-2 antigens (lateral flow devices). *GOV.UK* https://www.gov.uk/government/publications/assessment-and-procurement-of-coronavirus-covid-19-tests/protocol-for-evaluation-of-rapid-diagnostic-assays-for-specific-sars-cov-2-antigens-lateral-flow-devices.
17. Eyre, D. W. *et al.* Differential occupational risks to healthcare workers from SARS-CoV-2 observed during a prospective observational study. *eLife* **9**, e60675 (2020).
18. Gremmels, H. *et al.* Real-life validation of the Panbio™ COVID-19 antigen rapid test (Abbott) in community-dwelling subjects with symptoms of potential SARS-CoV-2 infection. *EClinicalMedicine* **0**, (2020).
19. Merino-Amador, P. *et al.* Multicenter evaluation of the Panbio™ COVID-19 Rapid Antigen-Detection Test for the diagnosis of SARS-CoV-2 infection. *medRxiv* 2020.11.18.20230375 (2020) doi:10.1101/2020.11.18.20230375.
20. Singanayagam, A. *et al.* Duration of infectiousness and correlation with RT-PCR cycle threshold values in cases of COVID-19, England, January to May 2020. *Eurosurveillance* **25**, 2001483 (2020).
21. Antigen-based testing but not real-time PCR correlates with SARS-CoV-2 virus culture | medRxiv. https://www.medrxiv.org/content/10.1101/2020.10.02.20205708v1.

medRxiv preprint doi: https://doi.org/10.1101/2021.01.13.21249563; this version posted January 15, 2021. The copyright holder for this preprint (which was not certified by peer review) is the author/funder, who has granted medRxiv a license to display the preprint in perpetuity. All rights reserved. No reuse allowed without permission.

22. Cevik, M. *et al.* SARS-CoV-2, SARS-CoV, and MERS-CoV viral load dynamics, duration of viral shedding, and infectiousness: a systematic review and meta-analysis. *Lancet Microbe* **0**, (2020).
23. Madewell, Z. J., Yang, Y., Longini, I. M., Halloran, M. E. & Dean, N. E. Household transmission of SARS-CoV-2: a systematic review and meta-analysis of secondary attack rate. *MedRxiv Prepr. Serv. Health Sci.* (2020) doi:10.1101/2020.07.29.20164590.
24. Nicol, T. *et al.* Assessment of SARS-CoV-2 serological tests for the diagnosis of COVID-19 through the evaluation of three immunoassays: Two automated immunoassays (Euroimmun and Abbott) and one rapid lateral flow immunoassay (NG Biotech). *J. Clin. Virol.* **129**, 104511 (2020).
25. Igl□i, Z. *et al.* Clinical evaluation of the Roche/SD Biosensor rapid antigen test with symptomatic, non-hospitalized patients in a municipal health service drive-through testing site. *medRxiv* 2020.11.18.20234104 (2020) doi:10.1101/2020.11.18.20234104.
26. Pilarowski, G. *et al.* Performance characteristics of a rapid SARS-CoV-2 antigen detection assay at a public plaza testing site in San Francisco. *medRxiv* 2020.11.02.20223891 (2020) doi:10.1101/2020.11.02.20223891.
27. Schwob, J.-M. *et al.* Antigen rapid tests, nasopharyngeal PCR and saliva PCR to detect SARS-CoV-2: a prospective comparative clinical trial. *medRxiv* 2020.11.23.20237057 (2020) doi:10.1101/2020.11.23.20237057.
28. Linares, M. *et al.* Panbio antigen rapid test is reliable to diagnose SARS-CoV-2 infection in the first 7 days after the onset of symptoms. *J. Clin. Virol.* **133**, 104659 (2020).
29. Bulilete, O. *et al.* Evaluation of the Panbio™ rapid antigen test for SARS-CoV-2 in primary health care centers and test sites. *medRxiv* 2020.11.13.20231316 (2020) doi:10.1101/2020.11.13.20231316.
30. Mak, G. C. *et al.* Evaluation of rapid antigen test for detection of SARS-CoV-2 virus. *J. Clin. Virol. Off. Publ. Pan Am. Soc. Clin. Virol.* **129**, 104500 (2020).
31. The effectiveness of population-wide, rapid antigen test based screening in reducing SARS-CoV-2 infection prevalence in Slovakia. *CMMID Repository* https://cmmid.github.io/topics/covid19/Slovakia.html (2020).
32. Boseley, S. & Elgot, J. Liverpool to pioneer UK's first attempt at mass Covid testing. *The Guardian* (2020).
33. Carmo, A. *et al.* Clearance and persistence of SARS-CoV-2 RNA in patients with COVID-19. *J. Med. Virol.* **92**, 2227–2231 (2020).
34. La Scola, B. *et al.* Viral RNA load as determined by cell culture as a management tool for discharge of SARS-CoV-2 patients from infectious disease wards. *Eur. J. Clin. Microbiol. Infect. Dis.* **39**, 1059–1061 (2020).
35. Mina, M. J., Parker, R. & Larremore, D. B. Rethinking Covid-19 Test Sensitivity — A Strategy for Containment. *N. Engl. J. Med.* **0**, null (2020).
36. Larremore, D. B. *et al.* Test sensitivity is secondary to frequency and turnaround time for COVID-19 surveillance. *medRxiv* (2020) doi:10.1101/2020.06.22.20136309.
37. Covid-19: Daily coronavirus test plan to cut contacts' 14-day self-isolation. *BBC News* (2020).
38. November 2020, J. S. NHS staff to get twice-weekly home covid tests with immediate effect. *Health Service Journal* https://www.hsj.co.uk/acute-care/nhs-staff-to-get-twice-weekly-home-covid-tests-with-immediate-effect/7028943.article.

medRxiv preprint doi: https://doi.org/10.1101/2021.01.13.21249563; this version posted January 15, 2021. The copyright holder for this preprint (which was not certified by peer review) is the author/funder, who has granted medRxiv a license to display the preprint in perpetuity. All rights reserved. No reuse allowed without permission.

Research in Context

Evidence before the study:

Lateral flow devices are a new form of testing for SARS-CoV-2. They differ from RT-PCR tests in that they rely on the detection of viral antigens by immunoassays and their utility has not yet been fully defined. A literature review was performed in PubMed and bioRxiv/medRxiv for all studies using lateral flow devices for the detection of SARS-CoV-2 viral antigen. This used the search terms “COVID-19”, “SARS-CoV-2”, “viral antigen” and “lateral flow devices” and was not limited to English language publications. To date, the majority of studies have been largely single centre studies analysing a single test and there are contrasting results with some LFDs showing good sensitivity and specificity[24 25 13 19 26 27 18], and others demonstrating poorer performance.[28 29]

Added value of the study

This UK COVID-19 Lateral Flow Oversight group study is the largest national evaluation undertaken of viral antigen LFDs for COVID-19. We have flagged four LFDs with the best performance characteristics from our assessments. The Innova LFD has been tested the most extensively and has high specificity with acceptable sensitivity. Our data has also highlighted the critical importance of training. We also note the need for further clinical studies to demonstrate that the identification of individuals with higher viral loads will be of benefit in interrupting transmission.

Implications of all the available evidence

Our data indicates that LFDs for COVID-19 have performance characteristics attractive for the UK mass testing program. Ongoing iterative evaluation of the population-level roll-out of LFDs in reducing transmission of COVID-19, and the contribution of such tests to reducing the risk of morbidity and mortality for clinically vulnerable individuals, is desirable. Further work is required to determine the amount and content of “training” to derive optimal test performance.

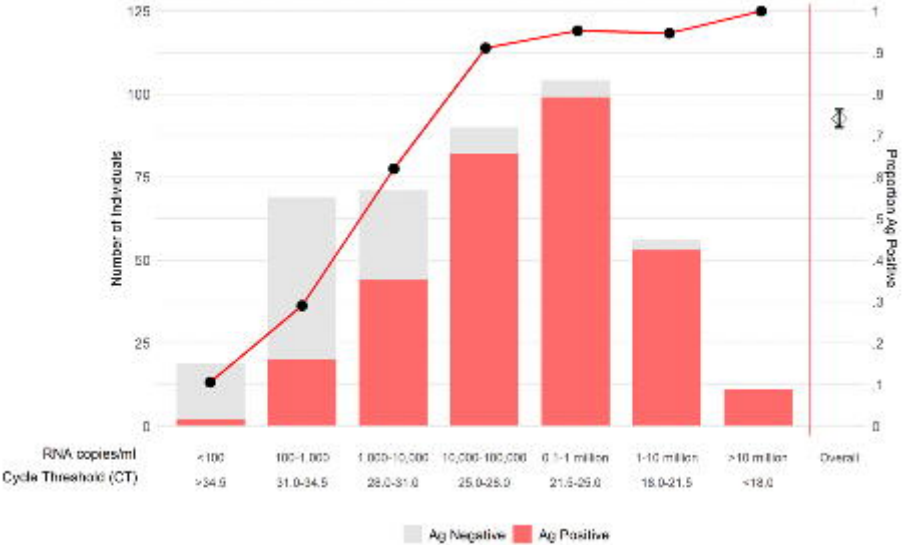
Number of Individuals
Proportion Ag Positive
125
100
75
50
25
0
1
.9
.8
.7
.6
.5
.4
.3
.2
.1
0
RNA copies/ml
Cycle Threshold (CT)
<100
>34.0
100-1,000
31.0-34.5
1,000-10,000
28.0-31.0
10,000-100,000
25.0-28.0
0.1-1 million
21.5-25.0
1-10 million
18.0-21.5
>10 million
<18.0
Overall
Ag Negative
Ag Positive

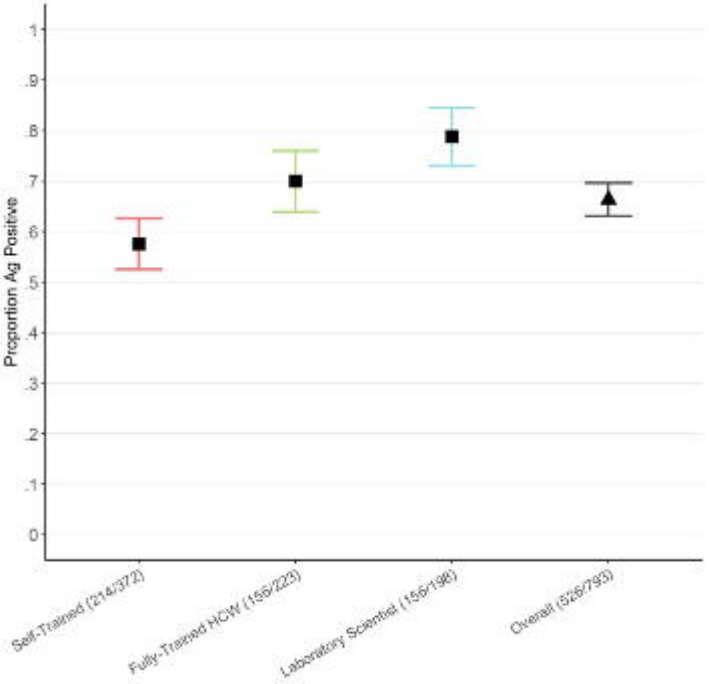
Proportion Ag Positive
1
.9
.8
.7
.6
.5
.4
.3
.2
.1
0
Self-Trained (214/372)
Fully-Trained HCW (159/223)
Laboratory Scientist (156/196)
Overall (528/793)