medRxiv preprint doi: https://doi.org/10.1101/2021.07.04.21259490; this version posted July 6, 2021. The copyright holder for this preprint (which was not certified by peer review) is the author/funder, who has granted medRxiv a license to display the preprint in perpetuity. All rights reserved. No reuse allowed without permission.

Generation of false positive SARS-CoV-2 antigen results with testing conditions outside manufacturer recommendations: A scientific approach to pandemic misinformation

Glenn Patriquin[1,2], Ross J. Davidson[1-4], Todd F. Hatchette[1-4], Breanne M. Head[5], Edgard Mejia[5], Michael G. Becker[5], Adrienne Meyers[5], Paul Sandstrom[5], Jacob Hatchette[6], Ava Block[6], Nicole Smith[6], John Ross[6], Jason J. LeBlanc[1-4*]

[1]Division of Microbiology, Department of Pathology and Laboratory Medicine, Nova Scotia Health (NSH), Halifax, Nova Scotia, Canada.

[2]Department of Pathology, Dalhousie University, Halifax, Nova Scotia, Canada.

[3]Department of Medicine (Infectious Diseases), Dalhousie University, Halifax, Nova Scotia, Canada.

[4]Department of Microbiology and Immunology, Dalhousie University, Halifax, Nova Scotia, Canada.

[5]National Microbiology Laboratory (NML), Public Health Agency of Canada (PHAC), Winnipeg, Manitoba, Canada.

[6]Praxes Medical Group, Halifax, Nova Scotia, Canada.

Key Words: COVID-19, SARS-CoV-2, antigen, false positive, Panbio

Abstract word count: 250

Body word count: 2989

***Corresponding author:** Jason J. LeBlanc, PhD, FCCM, D(ABMM)
Division of Microbiology, Department of Pathology and Laboratory Medicine, Nova Scotia Health (NSH),
Room 404B, MacKenzie Building
5788 University Avenue, Halifax, Nova Scotia, B3H 1V8
Tel.: +1 902 473 7698; Fax: +1 902 473 7971
Email: jason.leblanc@nshealth.ca

NOTE: This preprint reports new research that has not been certified by peer review and should not be used to guide clinical practice.

medRxiv preprint doi: https://doi.org/10.1101/2021.07.04.21259490; this version posted July 6, 2021. The copyright holder for this preprint (which was not certified by peer review) is the author/funder, who has granted medRxiv a license to display the preprint in perpetuity. All rights reserved. No reuse allowed without permission.

Abstract

Objectives. Antigen-based rapid diagnostics tests (Ag-RDTs) are useful tools for SARS-CoV-2 detection. However, misleading demonstrations of the Abbott Panbio COVID-19 Ag-RDT on social media claimed that SARS-CoV-2 antigen could be detected in municipal water and food products. To offer a scientific rebuttal to pandemic misinformation and disinformation, this study explored the impact of using the Panbio SARS-CoV-2 assay with conditions falling outside of manufacturer recommendations.

Methods. Using Panbio, various water and food products, laboratory buffers, and SARS-CoV-2-negative clinical specimens were tested, with and without manufacturer buffer. Additional experiments were conducted to assess the role of each Panbio buffer component (tricine, NaCl, pH, and tween-20), as well as the impact of temperatures (4°C, 20°C , and 45°C) and humidity (90%) on assay performance.

Results. Direct sample testing (without the kit buffer), resulted in false positive signals resembling those obtained with SARS-CoV-2-positive controls tested under proper conditions. The likely explanation of these artifacts is non-specific interactions between the SARS-CoV-2-specific conjugated and capture antibodies, as proteinase K treatment abrogated this phenomenon, and thermal shift assays showed pH-induced conformational changes under conditions promoting artifact formation. Omitting, altering, and reverse engineering the kit buffer all supported the importance of maintaining buffering capacity, ionic strength, and pH for accurate kit function. Interestingly, the Panbio assay could tolerate some extremes of temperature and humidity outside of manufacturer claims.

Conclusions. Our data support strict adherence to manufacturer instructions to avoid false positive SARS-CoV-2 Ag-RDT reactions, otherwise resulting in anxiety, overuse of public health resources, and dissemination of misinformation.

medRxiv preprint doi: https://doi.org/10.1101/2021.07.04.21259490; this version posted July 6, 2021. The copyright holder for this preprint (which was not certified by peer review) is the author/funder, who has granted medRxiv a license to display the preprint in perpetuity. All rights reserved. No reuse allowed without permission.

Introduction

High demand for diagnostic testing during the COVID-19 pandemic led to the development of various technologies for SARS-CoV-2 detection.[1] Nucleic acid amplification tests (NAATs), like real-time RT-PCR, are considered the reference methods [2-4], but antigen-based rapid diagnostic tests (Ag-RDTs) have been widely used due to their ease-of use, rapid results, and ability to be performed outside of a laboratory setting.[1] Many Ag-RDTs have been licensed as point-of-care (POC) devices for SARS-CoV-2 detection [5,6], but their performance can vary between methods, testing frequency, and settings in which they are used.[7-13] Ag-RDTs are well recognized to be less sensitive and specific than commercial NAATs, and false positive results from Ag-RDTs are known to occur, particularly in settings of low disease prevalence.[14,15]

Recently, misleading demonstrations of a SARS-CoV-2 Ag-RDT (i.e. Panbio) on social media platforms have claimed that SARS-CoV-2 antigen can readily be detected in municipal water and commercial food and beverages; however, direct testing of samples onto Ag-RDTs devices is not recommended by the manufacturer. With misinformation and disinformation often perpetuated on social media, unsubstantiated claims can undermine confidence in SARS-CoV-2 diagnostic testing and erode trust in public health efforts. As such, it is important to use science-based approaches to demonstrate that non-specific reactivity can occur when testing is performed under inappropriate conditions, and that SARS-CoV-2 is not truly present in food or potable water samples. This study evaluated conditions that fell outside of those recommended by the manufacturer, which had the potential to generate aberrant Ag-RDT reactions, including unregulated buffering capacity or ionic strength, and extremes of temperature, humidity, and pH.

Materials and methods

Samples types

medRxiv preprint doi: https://doi.org/10.1101/2021.07.04.21259490; this version posted July 6, 2021. The copyright holder for this preprint (which was not certified by peer review) is the author/funder, who has granted medRxiv a license to display the preprint in perpetuity. All rights reserved. No reuse allowed without permission.

Ag-RDT samples included food products (Table S1), water, laboratory buffers, specimen transport media, and 30 each of four different clinical specimens types: 1) nasopharyngeal (NP) swabs in universal transport media (UTM); 2) oropharyngeal and bilateral nares (OP/N) swabs in phosphate buffered saline (PBS) [16,17]; 3) bronchoalveolar lavages (BAL); and 4) saline gargles (Table 1).[18,19]

Antigen and molecular testing

SARS-CoV-2 nucleocapsid antigen detection was performed using the Abbott Panbio COVID-19 Rapid Antigen Test and the BD Veritor System for Rapid Detection of SARS-CoV-2. Each kit's nasal swabs were dipped into the test samples, placed in the appropriate kit buffers, and 3 or 5 drops were used to inoculate the sample wells of the Veritor and Panbio cassettes, respectively, as per the manufacturer recommendations. Each sample was also tested without manufacturer buffer (i.e. direct sample testing), mirroring the procedure and volume recommended for buffer. Results were visualized by the unaided eye after 15 minutes, and Veritor readouts also included automated detection using a BD Veritor Plus instrument. Real-time RT-PCR testing was performed for all specimens except food products using the Roche Diagnostics cobas SARS-CoV-2 Test on the cobas 6800 instrument.

Assessing Panbio buffer components

The exact composition of Panbio buffer is proprietary, yet according to the product insert, it consists of tricine, sodium chloride (NaCl), tween-20, proclin 300, and sodium azide (<0.1%). To assess the role of these components, the buffer was reverse engineered. PCR-grade water (Invitrogen) was chosen as a representative matrix to generate false positive Panbio results (Table 1). Solutions of tricine (1 mM to 1M), from pH 3 to 12 were prepared (Figure 1), with or without 1% tween-20. The contribution of ionic strength was assessed using NaCl (1 mM to 1M) in 100 mM tricine solutions pH 3 to 12 (Figure 2).

medRxiv preprint doi: https://doi.org/10.1101/2021.07.04.21259490; this version posted July 6, 2021. The copyright holder for this preprint (which was not certified by peer review) is the author/funder, who has granted medRxiv a license to display the preprint in perpetuity. All rights reserved. No reuse allowed without permission.

Effect of temperature and humidity on Ag-RDT performance

Dilutions of gamma-irradiated SARS-CoV-2 were assessed at pre-treatment and operational temperatures within (20°C), below (4°C), or above [45°C, 90% relative humidity (RH)] the recommended test conditions (Document S1 and Table S2). Additional experiments evaluated freezing Panbio test components at -20°C, or long-term incubation (16h) at high humidity and temperature (Document S1). To assess the limit of tolerance to water-induced artifacts, Panbio buffer was serially diluted and tested at 4°C, 20°C, and 37°C (Figure 3).

Investigation of environmental conditions on PanBio performance

According to manufacturer specifications, PanBio kits should be stored between 2 to 30 °C, and all kit components brought to room temperature (15 to 30 °C) for 30 minutes prior to use. To assess the impact of storage temperature, sealed PanBio test devices were incubated for one hour at 4°C, 20°C or 45°C (with 90% relative humidity using a Binder Constant Climate Chamber model KBF 115). Test devices were removed from their packaging, and incubations were repeated under the same conditions. Testing was performed using 20 µL of gamma-irradiated SARS-CoV-2 into 280 µL of PanBio buffer. Viral stocks [at 1.2×10^6 plaque forming units (PFU)/mL] were diluted in PBS (pH = 7.4) to concentrations spanning 1.2×10^5 to 1.1×10^3 PFU/mL (Supplemental Table S2). PanBio buffer and PBS were used as negative controls. Freeze-thaw effects were investigated by incubation of test components at -20°C for 16 hours before thawing and testing. Long-term exposure to high temperature and humidity was investigated by removing test components from packaging and subjecting them to 16 hours at 45°C (with 90% relative humidity).

Investigations into possible causes of false positive results

medRxiv preprint doi: https://doi.org/10.1101/2021.07.04.21259490; this version posted July 6, 2021. The copyright holder for this preprint (which was not certified by peer review) is the author/funder, who has granted medRxiv a license to display the preprint in perpetuity. All rights reserved. No reuse allowed without permission.

Using "conjugate pad transplantation" (Figure S1), the proprietary gold conjugated-antibodies of the Panbio device (i.e. the SARS-CoV-specific human IgG and the chicken IgY used for the control) were accessed from disassembled Panbio cassettes. Each conjugate pad was resuspended with 100 µl of Panbio buffer, PCR-grade water, or tricine solutions, and the suspensions were subjected to various treatments. Proteinase K (PK) (Qiagen GmbH., Hilden, Germany) was used at 100 µg/reaction for one hour at 56°C, followed by enzyme inactivation at 70°C for 10 minutes. Untreated and heat treatment controls were included as controls (Figure S2). The remaining conjugate-free pads are washed three times with 1 ml of water or buffer, dried using a Whatman #1 filter, and re-introduced into the Panbio cassettes. For testing, 25 µl of each water- or buffer-derived conjugated-antibody suspension was added onto the conjugate pads of reassembled cassettes, followed by addition of 5 drops into the sample well of either positive or negative controls processed in water or the kit buffer.

In a second set of experiments (Figure S1, dashed lines), the control chicken IgG was removed from the SARS-CoV-2-specific IgG by pre-treatment of the conjugate suspensions with a fragment of the nitrocellulose membrane from the Panbio test device containing the immobilized mouse monoclonal anti-chicken IgY. Fragments were excised at approximately 3 mm on each side of the control line indicated on the Panbio cassette. For each 100 µl of conjugate suspension, one fragment was added, followed by a 15 min incubation at room temperature. Then, SARS-CoV-2-specific conjugated antibody were removed and subjected to thermal shift assays [20-22] to explore possible pH-induced conformational changes (Figure S3).

Conjugated SARS-CoV-2 IgG thermal shift assays

Differential scanning fluorometry (DSF), also known as thermal shift assays, relies on monitoring temperature-dependent unfolding of a protein, in presence of a fluorescent dye that is quenched in water but fluoresces when bound to hydrophobic residues.[20-22] As a native protein is unfolded with

medRxiv preprint doi: https://doi.org/10.1101/2021.07.04.21259490; this version posted July 6, 2021. The copyright holder for this preprint (which was not certified by peer review) is the author/funder, who has granted medRxiv a license to display the preprint in perpetuity. All rights reserved. No reuse allowed without permission.

heat, different hydrophobic residues are exposed, and the melting temperature (Tm) can be calculated for various test conditions. In this study, 25 µl reaction containing 10× SYPRO Orange (Invitrogen, Eugene, Oregon, USA) was added to the gold-conjugated human IgG specific to SARS-CoV-2 resuspended in Panbio buffer or 100 mM of tricine at pH values spanning 3 to 12, with or without 1% tween-20. Melting curve analysis was performed by increasing the temperature from 25°C to 99.9°C at a ramp rate of 1% with continuous fluorescence at 610 nm using an Applied Biosystems 7500 Fast instrument. Tm values were calculated by manufacturer software (Figure S3).

Results

False positives in food, water, buffers, media, and clinical specimens

With the exception of soft drinks and some milk products which produced negative or weak false positive reactions, most of the food products that were tested directly onto the Panbio cassette produced a strong positive SARS-CoV-2 signals that resembled those obtained with the kit positive control (Table S1). Direct testing of highly acidic samples caused invalid results for both Panbio and Veritor. All other products were Veritor-negative. When nasal swabs were used to sample the various products and processing occurred with manufacturer buffer, no false positives or invalid results were observed.

Multiple water samples were evaluated with tested pH values between 4.00 and 9.33, and differences in supplier-described purification methods, and mineral and electrolyte composition (Table 1). Direct testing onto Panbio test devices showed strong false positive SARS-CoV-2 signals, while samples diluted in Panbio buffer did not produce any artifacts. Notably, water samples near the pH of the Panbio buffer (pH 8.78) also displayed strong false positive signals, suggesting the mechanism behind artifact formation is not, or not solely, pH-dependent. To investigate the possible roles of buffering capacity and ionic strength, commonly used laboratory buffers and buffer-containing viral transport media spanning

medRxiv preprint doi: https://doi.org/10.1101/2021.07.04.21259490; this version posted July 6, 2021. The copyright holder for this preprint (which was not certified by peer review) is the author/funder, who has granted medRxiv a license to display the preprint in perpetuity. All rights reserved. No reuse allowed without permission.

various pH values (5.62 to 8.78) were tested (Table 1). With the exception of Tris-EDTA (TE), all other buffers and media generated weakly positive or negative results (Table 1). All water samples, buffers, and media were RT-PCR and Veritor-negative, suggesting absence of viral RNA and nucleocapsid antigen, respectively (Table 1).

Given that weak false positive were results observed with UTM, PBS, and saline, direct testing was performed on clinical specimens containing these media and buffers. With direct testing onto Panbio cassettes, false positive results were seen in 93.3% of NP swabs in UTM, 86.7% of OP/N swabs in PBS, 90.0% of BALs, and 90.0% of the saline gargles (Table 1). All specimens were negative when Panbio buffer was used, which was consistent with the Veritor and RT-PCR results.

Role of Panbio buffer components

Tricine solutions at 1M prevented artifact formation at pH values ≥7, whereas strong false positive SARS-CoV-2 results were seen at pH ≤ 5 (Figure 1). At 100 mM tricine, buffering capacity was narrowed, and non-specific SARS-CoV-2 bands were seen at pH ≤ 8. With the exception of invalid results obtained at pH 3 and 12, false positive results at either 1 or 10 mM of tricine when pH ranged between 4 and 11. Tween-20 (1%) was added to all tricine solutions, but had no impact on results (data not shown). Ionic strength was assessed with various NaCl concentrations in 100 mM tricine solutions, pH 3 to 12 (Figure 2). High concentration of NaCl (1M) prevented artifact formation, 100 mM reduced it, and lower concentrations (1 and 10 mM) mirrored NaCl-free conditions (Figure 1 and 2). Antimicrobial agents in the Panbio buffer (i.e. proclin 300 and sodium azide) were not investigated due to their unlikely contribution to artifact generation.

Investigations into the mechanism of artifact generation

medRxiv preprint doi: https://doi.org/10.1101/2021.07.04.21259490; this version posted July 6, 2021. The copyright holder for this preprint (which was not certified by peer review) is the author/funder, who has granted medRxiv a license to display the preprint in perpetuity. All rights reserved. No reuse allowed without permission.

Following conjugate pad transplantation, positive and negative control swabs displayed expected results after inoculation onto re-assembled Panbio cassettes in which resuspended conjugated antibodies were re-introduced. Water-resuspended conjugated antibody generated a strong false positive target signal, which was eliminated following PK treatment (Figure S2). Removal of the gold-conjugated IgY antibody from the conjugate suspensions did not impair Panbio test performance, and the strong false positive SARS-CoV-2 signal from water remained (Figure S2). These findings suggest that the gold-conjugated human anti-SARS-CoV-2 IgG is responsible for the non-specific interactions with the immobilized anti-SARS-CoV-2 capture antibody on the test device nitrocellulose membrane. Thermal shift assays in 100 mM tricine solutions were used to compare structural differences of the anti-SARS-CoV-2 IgG at different pH (Figure S3), and Tm values were significantly different in tricine solutions between pH 5 to 7 (at 68.4 ± 2.6, 71.4 ± 1.2, 72.5 ± 1.0, respectively) compared to pH 8 to 10 (at 75.6 ± 1.0, 76.8 ± 1.1 and 77.6 ± 1.4, respectively) (Figure S3). Tm values at pH 4 and 11 were inconsistent, while no Tm values could be established at pH 3 and 12.

Impact of heat and humidity on Panbio kit function

In all test conditions evaluated (Table S1), no deleterious effects on test sensitivity or specificity were observed concerning temperature or humidity. In a complimentary series of experiments, Panbio buffer was able to tolerate dilutions with water (without generating artifacts) up to a ratio of 1:10, regardless of operating temperature (Figure 3).

Discussion

False positive and negative results occur with any diagnostic test, but are increasingly likely when manufacturer recommendations are not followed.[1,14,15] Using the Panbio SARS-CoV-2 Ag-RDT, this study demonstrated test conditions outside manufacturer recommendations that can cause false positive results. In absence of manufacturer buffer, a variety of food, water, laboratory buffer, specimen

medRxiv preprint doi: https://doi.org/10.1101/2021.07.04.21259490; this version posted July 6, 2021. The copyright holder for this preprint (which was not certified by peer review) is the author/funder, who has granted medRxiv a license to display the preprint in perpetuity. All rights reserved. No reuse allowed without permission.

transport media, and clinical specimens showed false positive reactions. Uncontrolled conditions of pH, buffering capacity, and ionic strength, all favored artifact generation, whereas temperature and humidity were not contributory under the tested parameters.

The principal components of the Panbio buffer, tricine and NaCl, were shown to help maintain buffering capacity, ionic strength, and pH compatible with the proper function of the assay. Panbio buffer diluted in water at ratios greater than 1:10 resulted in artifact formation. Similarly, when buffering capacity was poor or lost when using low tricine concentrations (1 or 10 mM), strong false positive signals were seen across a broad range of pH values. In contrast, high tricine concentrations (100 mM or 1M) prevented artifact formation at pH 9 and above, which is consistent with the measured pH of Panbio buffer at 8.78. Similarly, regulated ionic strength also played an important role, as high NaCl concentrations (100 mM or 1M) reduced or prevented false positive results. Of note, strong artifacts were generated with most food and water samples, due to their poor buffering capacity and ionic strength, whereas only weak positive or negative results seen with buffers, media, and clinical specimens. These data are consistent with others [23] who recognized the importance of Ag-RDT kit buffers.

Other possible explanations for false positive Ag-RDT results include cross-reactions [24], interfering substances [25,26], and improper operating or storage conditions for temperature or humidity.[27]. Cross-reacting or interfering substances common to all samples tested in the study is unlikely. Temperature extremes have been shown to induce conformational changes in antibodies leading to non-specific binding [28]; however, in this study, Panbio was unaffected by temperature and humidity. As mentioned above, the most likely cause of Panbio false positive results was aberrant protein-protein interactions faced with improper buffer conditions, ionic strength, or pH.

In a previous study, 20 of 27 of the malaria Ag-RDTs brands evaluated showed false positive reactions when the manufacturer buffer was replaced with saline, tap water, or distilled water.[23] Distilled water

medRxiv preprint doi: https://doi.org/10.1101/2021.07.04.21259490; this version posted July 6, 2021. The copyright holder for this preprint (which was not certified by peer review) is the author/funder, who has granted medRxiv a license to display the preprint in perpetuity. All rights reserved. No reuse allowed without permission.

alone generated false positive reactions [23], similar to what was observed in this study with Panbio. Possible explanations for their findings included inefficient resuspension of blocking agents, altered capillary flow rates and decreased flushing of contaminating substances, and finally, non-specific interactions between the conjugated and capture antibodies faced with uncontrolled buffering and ionic strength conditions.[23] Tricine is a zwitterionic amino acid with a pKa of 8.26, and in the Panbio buffer, would be negatively charged at the measured pH of 8.78. Therefore, under recommended testing conditions, tricine may mask positively charged residues on the SARS-CoV-2-specific conjugated and capture antibodies, while uncontrolled buffer conditions would favor aberrant electrostatic or hydrophobic interactions between the two antibodies, resulting in false positive results. Supporting this theory, PK treatment eliminated the false positive Panbio results generated by water, and the propensity to generate this artifact varied with buffering capacity, pH, and ionic strength. Removal of the gold-conjugated chicken IgY (used for control band detection) did not alter formation of the SARS-CoV-2 target artifact formation, suggesting the SARS-CoV-2-specific conjugated IgG alone is responsible for non-specific binding and to the SARS-CoV-2-specific capture antibody and artifact formation. Finally, thermal shift assays were performed on the conjugated anti-SARS-CoV-2 IgG, and pH-dependent conformation changes were observed under conditions causing false positive results.

False positive reactions with the Panbio Ag-RDT have the potential to cause a significant impact to Public Health. To date, over 200 million Panbio Ag-RDT tests have been distributed to over 120 countries worldwide, for use in healthcare settings, businesses, or home self-testing. In low prevalence populations, positive Ag-RDTs are typically confirmed by clinical laboratories with NAATs, thereby limiting the overall public health impact of the possible artifacts described in this study.[2-4] However, in programs where home self-testing kits are deployed, it is important to educate users on the importance of strict adherence to manufacturer instructions. Such education could prevent overuse of public health and laboratory resources required to investigate false positive reactions, and may alleviate anxieties for

medRxiv preprint doi: https://doi.org/10.1101/2021.07.04.21259490; this version posted July 6, 2021. The copyright holder for this preprint (which was not certified by peer review) is the author/funder, who has granted medRxiv a license to display the preprint in perpetuity. All rights reserved. No reuse allowed without permission.

the impacted individuals.[17,19,29,30] Another area for consideration is outdoor testing strategies (e.g. drive-thru testing), where the Panbio kit supplies may be exposed to precipitation and fluctuations in temperature and humidity.[30] To reduce potential aberrant results from humidity, each Panbio cassette is packaged with a desiccant; however, hypothetically, once opened, the accumulation of moisture in humid environments could cause false positive results. Prolonged exposure to elevated temperatures has been shown to affect the sensitivity of SARS-CoV-2 detection by Ag-RDTs, whereas low temperatures impaired specificity.[25] This could potentially impact Ag-RDT programs in countries where extreme environmental conditions are relevant, particularly in those where access to NAAT-based confirmatory testing is limited. While temperature and humidity did not alter the Panbio performance in this study, rain water was shown to cause false positive reactions if processed without buffer. An alternative explanation for the false positives observed at low temperatures by Haage et al [25] is their use of non-validated specimen types (i.e. NP swabs in PBS). In this study, PBS alone caused false positive results in absence of buffer, as did most of the saline-based clinical specimens. While PBS could be a contributing factor in the generation of false positive results, the quantity of PBS material (i.e. 20 µl) used by Haage et al.[25] should not have overwhelmed the kit buffer, as this study demonstrated tolerance to dilution up to a ratio of 1:10.

Overall, this manuscript provides rigorous scientific evidence that erroneous false positive SARS-CoV-2 results can occur with improper test conditions, resulting in non-specific interaction between the SARS-CoV-2-specific conjugated and capture antibodies. As such, SARS-CoV-2 Ag-RDTs should not deviate from manufacturer instructions.

Acknowledgement

The authors would like to thank the Special Pathogens Program of the National Microbiology Laboratory (NML) (Winnipeg, MB) for the gamma-irradiated SARS-CoV-2 virus used in this study. We would also like

medRxiv preprint doi: https://doi.org/10.1101/2021.07.04.21259490; this version posted July 6, 2021. The copyright holder for this preprint (which was not certified by peer review) is the author/funder, who has granted medRxiv a license to display the preprint in perpetuity. All rights reserved. No reuse allowed without permission.

to recognize the ongoing efforts of the all the NML and NSH staff for their dedication and exceptional services throughout the pandemic, including the help with RT-PCR testing during this evaluation. The authors would also like to thank all the volunteers and healthcare professionals who dedicate their time at popup clinics that use Ag-RDTs. You are all instrumental for our pandemic responses, and safety in our communities.

Author contributions

JH, AB, NS, and JR identified this phenomenon, and were involved in food sample testing. JL, RD, GP, and TH designed and undertook testing of water, buffer, media, and gargles. JL designed and performed the buffer reverse engineering, conjugate pad transplantation, PK experiments and DSF experiments. MB, AM, EM, BH, and PS designed and performed the temperature and humidity experiments. GP, JL, and TH wrote the initial draft of the manuscript, with all authors contributing to the final version.

Transparency declaration

The authors declare that they have no conflicts of interest. This work received no private or public funding, with the exception of the Panbio kits that were provided in-kind from the Public Health Agency of Canada (PHAC).

Ethics

This evaluation was deemed exempt from Nova Scotia Health Research Ethics Board approval, as the activities described in this manuscript were conducted in fulfillment of ongoing verification of SARS-CoV-2 diagnostic assays used in Nova Scotia, and are therefore considered a quality assurance initiative. Clinical specimens tested were obtained from anonymized residual samples collected for routine diagnostic testing for SARS-CoV-2 from consenting participants, and all data related to clinical specimens were provided anonymized, de-identified, and were used solely with the intent to evaluate the potential

medRxiv preprint doi: https://doi.org/10.1101/2021.07.04.21259490; this version posted July 6, 2021. The copyright holder for this preprint (which was not certified by peer review) is the author/funder, who has granted medRxiv a license to display the preprint in perpetuity. All rights reserved. No reuse allowed without permission.

for false positives in these clinical specimen types for rapid antigen testing programs used in Nova Scotia.

References

1. Safiabadi Tali SH, LeBlanc JJ, Sadiq Z, Oyewunmi OD, Camargo C, Nikpour B, Armanfard N, Sagan SM, Jahanshahi-Anbuhi S. 2021. Tools and techniques for severe acute respiratory syndrome coronavirus 2 (SARS-CoV-2)/COVID-19 detection. Clin Microbiol Rev. 34(3):e00228-20. doi: 10.1128/CMR.00228-20. PMID: 33980687.
2. Public Health Agency of Canada (PHAC). 2020. Interim guidance on the use of rapid antigen detection tests for the identification of SARS-CoV-2 infection. https://www.canada.ca/en/public-health/services/diseases/2019-novel-coronavirus-infection/guidance-documents/use-rapid-antigen-detection-tests.html (accessed June 21, 2021).
3. World Health Organization (WHO). 2020. Antigen-detection in the diagnosis of SARS-CoV-2 infection using rapid immunoassays. Interim guidance. https://www.who.int/publications/i/item/antigen-detection-in-the-diagnosis-of-sars-cov-2infection-using-rapid-immunoassays (accessed June 21, 2021)
4. Centers for Disease Control and Prevention (CDC). 2020. Interim guidance for antigen testing for SARS-CoV-2. https://www.cdc.gov/coronavirus/2019-ncov/lab/resources/antigen-tests-guidelines.html (accessed June 21, 2021).
5. US Food and Drug Administration. 2020. In vitro diagnostics EUAs. https://www.fda.gov/medical-devices/coronavirus-disease-2019-covid-19-emergency-use-authorizations-medical-devices/vitro-diagnostics-euas#individual-molecular (accessed June 21, 2021).

medRxiv preprint doi: https://doi.org/10.1101/2021.07.04.21259490; this version posted July 6, 2021. The copyright holder for this preprint (which was not certified by peer review) is the author/funder, who has granted medRxiv a license to display the preprint in perpetuity. All rights reserved. No reuse allowed without permission.

6. Health Canada. 2020. Authorized medical devices for uses related to COVID-19: List of authorized testing devices. https://www.canada.ca/en/health-canada/services/drugs-health-products/covid19-industry/medical-devices/authorized/list.html (accessed June 21, 2021).

7. Patriquin G, LeBlanc JJ. SARS-CoV-2 sensitivity limbo - How low can we go? Int J Infect Dis. 2021 Feb;103:23-24. doi: 10.1016/j.ijid.2020.11.138. Epub 2020 Nov 17. PMID: 33212261; PMCID: PMC7669480.

8. Merino P, Guinea J, Muñoz-Gallego I, González-Donapetry P, Galán JC, Antona N, Cilla G, Hernáez-Crespo S, Díaz-de Tuesta JL, Gual-de Torrella A, González-Romo F, Escribano P, Sánchez-Castellano MÁ, Sota-Busselo M, Delgado-Iribarren A, García J, Cantón R, Muñoz P, Folgueira MD, Cuenca-Estrella M, Oteo-Iglesias J; Spanish Panbio™ COVID-19 validation group. 2021. Multicenter evaluation of the Panbio COVID-19 rapid antigen-detection test for the diagnosis of SARS-CoV-2 infection. Clin Microbiol Infect. 27(5):758-61. doi: 10.1016/j.cmi.2021.02.001. Epub ahead of print. PMID: 33601009; PMCID: PMC7884234.

9. Scheiblauer H, Filomena A, Nitsche A, Puyskens A, Corman VM, Drosten C, Zwirglmaier K, Lange C, Emmerich P, Müller M, Knauer O, Nübling CM. 2021. Comparative sensitivity evaluation for 122 CE-marked SARS-CoV-2 antigen rapid tests. medRxiv 2021.05.11.21257016; doi: https://doi.org/10.1101/2021.05.11.21257016

10. Gremmels H, Winkel BMF, Schuurman R, Rosingh A, Rigter NAM, Rodriguez O, Ubijaan J, Wensing AMJ, Bonten MJM, Hofstra LM. 2021. Real-life validation of the Panbio COVID-19 antigen rapid test (Abbott) in community-dwelling subjects with symptoms of potential SARS-CoV-2 infection. EClinicalMedicine 31:100677. https://doi.org/10.1016/j.eclinm.2020.100677.

11. Linares M, Pérez-Tanoira R, Carrero A, Romanyk J, Pérez-García F, Gómez-Herruz P, Arroyo T, Cuadros J. 2020. Panbio antigen rapid test is reliable to diagnose SARS-CoV-2 infection in the first 7

medRxiv preprint doi: https://doi.org/10.1101/2021.07.04.21259490; this version posted July 6, 2021. The copyright holder for this preprint (which was not certified by peer review) is the author/funder, who has granted medRxiv a license to display the preprint in perpetuity. All rights reserved. No reuse allowed without permission.

days after the onset of symptoms. J Clin Virol. 133:104659. doi: 10.1016/j.jcv.2020.104659. Epub 2020 Oct 16. PMID: 33160179; PMCID: PMC7561603.

12. Albert E, Torres I, Bueno F, Huntley D, Molla E, Fernández-Fuentes MÁ, Martínez M, Poujois S, Forqué L, Valdivia A, Solano de la Asunción C, Ferrer J, Colomina J, Navarro D. 2021. Field evaluation of a rapid antigen test (Panbio COVID-19 Ag Rapid Test Device) for COVID-19 diagnosis in primary healthcare centres. Clin Microbiol Infect. 27(3):472.e7-472.e10. doi: 10.1016/j.cmi.2020.11.004. Epub 2020 Nov 13. PMID: 33189872; PMCID: PMC7662075.
13. Stokes W, Berenger BM, Portnoy D, Scott B, Szelewicki J, Singh T, Venner AA, Turnbull L, Pabbaraju K, Shokoples S, Wong AA, Gill K, Guttridge T, Proctor D, Hu J, Tipples G. 2021. Clinical performance of the Abbott Panbio with nasopharyngeal, throat, and saliva swabs among symptomatic individuals with COVID-19. Eur J Clin Microbiol Infect Dis. 20:1-6. doi: 10.1007/s10096-021-04202-9. Epub ahead of print. PMID: 33742322; PMCID: PMC7979467.
14. Food and Drug Administration (FDA). 2020. Potential for false positive results with antigen tests for rapid detection of SARS-CoV-2 - Letter to clinical laboratory staff and health care providers. https://www.fda.gov/medical-devices/letters-health-care-providers/potential-false-positive-results-antigen-tests-rapid-detection-sars-cov-2-letter-clinical-laboratory (accessed June 21, 2021).
15. Nikolayevskyy V, Drobniewski F. 2020. False-positive COVID-19 results: hidden problems and costs. Lancet Respir Med. 8(12):1167-1168. doi: 10.1016/S2213-2600(20)30453-7. Epub 2020 Sep 29. PMID: 33007240; PMCID: PMC7524437.
16. LeBlanc JJ, Heinstein C, MacDonald J, Pettipas J, Hatchette TF, Patriquin G. 2020. A combined oropharyngeal/nares swab is a suitable alternative to nasopharyngeal swabs for the detection of SARS-CoV-2. J Clin Virol. 128:104442. doi: 10.1016/j.jcv.2020.104442. Epub 2020 May 16. PMID: 32540034; PMCID: PMC7228872.

medRxiv preprint doi: https://doi.org/10.1101/2021.07.04.21259490; this version posted July 6, 2021. The copyright holder for this preprint (which was not certified by peer review) is the author/funder, who has granted medRxiv a license to display the preprint in perpetuity. All rights reserved. No reuse allowed without permission.

17. Patriquin G, Davis I, Heinstein C, MacDonald J, Hatchette TF, LeBlanc JJ. 2020. Exploring alternative swabs for use in SARS-CoV-2 detection from the oropharynx and anterior nares. J Virol Methods. 285:113948. doi: 10.1016/j.jviromet.2020.113948. Epub 2020 Aug 9. PMID: 32783913; PMCID: PMC7415171.

18. Goldfarb DM, Tilley P, Al-Rawahi GN, Srigley JA, Ford G, Pedersen H, Pabbi A, Hannam-Clark S, Charles M, Dittrick M, Gadkar VJ, Pernica JM, Hoang LMN. 2021. Self-collected saline gargle samples as an alternative to health care worker-collected nasopharyngeal swabs for COVID-19 diagnosis in outpatients. J Clin Microbiol. 59(4):e02427-20. doi: 10.1128/JCM.02427-20. PMID: 33514627.

19. LeBlanc JJ, Pettipas J, Di Quinzio M, Hatchette TF, Patriquin G. 2021. Reliable detection of SARS-CoV-2 with patient-collected swabs and saline gargles: A three-headed comparison on multiple molecular platforms. Journal of Virological Methods 295:114184. doi: 10.1016/j.jviromet.2021.114184. Epub ahead of print. PMID: 34029634; PMCID: PMC8141269.

20. Davey L, Cohen A, LeBlanc J, Halperin SA, Lee SF. 2016. The disulfide oxidoreductase SdbA is active in Streptococcus gordonii using a single C-terminal cysteine of the CXXC motif. Mol Microbiol. 99(2):236-53. doi: 10.1111/mmi.13227. Epub 2015 Oct 30. PMID: 26395460.

21. Gao K, Oerlemans R, Groves MR. 2020. Theory and applications of differential scanning fluorimetry in early-stage drug discovery. Biophys Rev. 12(1):85-104. doi: 10.1007/s12551-020-00619-2. Epub 2020 Jan 31. PMID: 32006251; PMCID: PMC7040159.

22. Ramu T, Prasad ME, Connors E, Mishra A, Thomassin JL, LeBlanc JJ, Rainey JK, Thomas NA. 2013. A novel C-terminal region within the multicargo type III secretion chaperone CesT contributes to effector secretion. J Bacteriol. 195(4):740-56. doi: 10.1128/JB.01967-12. Epub 2012 Dec 7. PMID: 23222727; PMCID: PMC3562101.

medRxiv preprint doi: https://doi.org/10.1101/2021.07.04.21259490; this version posted July 6, 2021. The copyright holder for this preprint (which was not certified by peer review) is the author/funder, who has granted medRxiv a license to display the preprint in perpetuity. All rights reserved. No reuse allowed without permission.

23. Gillet P, Mori M, Van den Ende J, Jacobs J. 2010. Buffer substitution in malaria rapid diagnostic tests causes false-positive results. Malar J. 9:215. doi: 10.1186/1475-2875-9-215. PMID: 20650003; PMCID: PMC3224932.

24. Wanji S, Amvongo-Adjia N, Njouendou AJ, Kengne-Ouafo JA, Ndongmo WP, Fombad FF, Koudou B, Enyong PA, Bockarie M. 2016. Further evidence of the cross-reactivity of the Binax NOW Filariasis ICT cards to non-Wuchereria bancrofti filariae: experimental studies with Loa loa and Onchocerca ochengi. Parasit Vectors. 9:267. doi: 10.1186/s13071-016-1556-8. PMID: 27151313; PMCID: PMC4858834.

25. Selby C. 1999. Interference in immunoassay. Ann Clin Biochem. 36(6):704-21. doi: 10.1177/000456329903600603. PMID: 10586307.

26. Nivin B, Zancocchio T. 2012. Cluster of false-positive influenza B virus rapid antigen test results in a New York City hospital. J Clin Microbiol. 50(9):3141. doi: 10.1128/JCM.01452-12. Epub 2012 Jun 20. PMID: 22718940; PMCID: PMC3421782.

27. Haage V, Ferreira de Oliveira-Filho E, Moreira-Soto A, Kühne A, Fischer C, Sacks JA, Corman VM, Müller MA, Drosten C, Drexler JF. 2021. Impaired performance of SARS-CoV-2 antigen-detecting rapid diagnostic tests at elevated and low temperatures. J Clin Virol. 138:104796. doi: 10.1016/j.jcv.2021.104796. Epub 2021 Mar 16. PMID: 33773413; PMCID: PMC7962993.

28. Lin J, Dai W, Li W, Xiao L, Luo T, Guo Y, Yang Y, Han Y, Zhu P, Wu Q, He B, Wu J, Xia X. 2021. Potential false-positive and false-negative results for COVID-19 IgG/IgM antibody testing after heat-inactivation. Front Med (Lausanne). 7:589080. doi: 10.3389/fmed.2020.589080. PMID: 33537325; PMCID: PMC7849051.

29. Wehrhahn MC, Robson J, Brown S, Bursle E, Byrne S, New D, Chong S, Newcombe JP, Siversten T, Hadlow N. 2020. Self-collection: An appropriate alternative during the SARS-CoV-2 pandemic. J Clin

medRxiv preprint doi: https://doi.org/10.1101/2021.07.04.21259490; this version posted July 6, 2021. The copyright holder for this preprint (which was not certified by peer review) is the author/funder, who has granted medRxiv a license to display the preprint in perpetuity. All rights reserved. No reuse allowed without permission.

Virol. 128:104417. doi: 10.1016/j.jcv.2020.104417. Epub 2020 May 4. PMID: 32403007; PMCID: PMC7198188.

30. Siegler AJ, Hall E, Luisi N, Zlotorzynska M, Wilde G, Sanchez T, Bradley H, Sullivan PS. 2020. Willingness to seek diagnostic testing for SARS-CoV-2 with home, drive-through, and clinic-based specimen collection locations. Open Forum Infect Dis. 7(7):ofaa269. doi: 10.1093/ofid/ofaa269. PMID: 32704517; PMCID: PMC7337815.

Figure legends

Figure 1. False positives SARS-CoV-2 Ag-RDT results can occur from uncontrolled pH and buffering conditions. All tricine solutions were prepared in PCR-grade water known to generate false positive signals when tested directly onto Panbio test devices.

Figure 2. Impact of ionic strength from NaCl on the presence of false positive SARS-CoV-2 signal generated by direct processing of PCR-grade water.

Figure 3. Tolerability of the Panbio buffer to artifact generation by PCR-grade water at different temperatures.

Figure S1. Conjugate pad transplantation to access and investigate properties of the proprietary Panbio conjugated antibodies. Each step was followed to as depicted leading to treatment of the conjugated antibodies with proteinase K (PK) or heat (T°C), and comparisons were made with untreated controls

medRxiv preprint doi: https://doi.org/10.1101/2021.07.04.21259490; this version posted July 6, 2021. The copyright holder for this preprint (which was not certified by peer review) is the author/funder, who has granted medRxiv a license to display the preprint in perpetuity. All rights reserved. No reuse allowed without permission.

(none). In some experiments (dashed arrows), the gold-conjugated antibody suspensions were pre-treated with the control antibody (mouse anti-chicken IgY) was used to purify the SARS-CoV-2-specific conjugated antibody (human IgG) for subsequent thermal shift assays.

Figure S2. Proteainase K treatment of the conjugated antibodies and removal of chicken IgY. A) Proteinase K (PK) treatment. Using conjugate pad transplantation, gold-conjugated antibody suspensions in Panbio buffer or water were treated for an hour with PK at 56°C, followed by heat inactivation of PK at 70°C for 10 min. Following re-introduction into Panbio cassettes of conjugated antibodies that were untreated (none), heat-treated (T°C), or PK-treated, water and a negative control swab, and with buffer with either a positive or negative control swab were added to the sample well. B) To purify the SARS-CoV-2-specific conjugated antibody (human IgG) from the conjugated antibody suspensions, a pre-incubation with the control antibody (mouse anti-chicken IgY) excised from the nitrocellulose membrane was performed. Untreated (none) or pre-treatment (-IgY) are depicted for reassembled Panbio cassettes inoculated with negative or positive control swabs processed in buffer or water.

Figure S3. Representative thermal shift profiles for Panbio SARS-CoV-2-specific conjugated antibody at different pH values in 100 mM tricine. Melt temperatures (Tm) are indicated for each curve.

Table 1. Samples tested by SARS-CoV-2 Ag-RDTs with and without manufacturer buffer.

Category	Brand	Description	Avg. pH (± SD)	Panbio result		Veritor result		RT-PCR result
				Sample, direct	Swab of sample in buffer	Sample, direct	Swab of sample in buffer	
Water samples	Sigma Life Sciences	Double processed,	4.00 (± 0.01)	POS	NEG	NEG	NEG	NEG

medRxiv preprint doi: https://doi.org/10.1101/2021.07.04.21259490; this version posted July 6, 2021. The copyright holder for this preprint (which was not certified by peer review) is the author/funder, who has granted medRxiv a license to display the preprint in perpetuity. All rights reserved. No reuse allowed without permission.

(n=24)		tissue culture water, sterile filtered						
	Montellier	Carbonated spring water	4.68 (± 0.00)	POS	NEG	NEG	NEG	NEG
	Invitrogen	UltraPure distilled water, Dnase- and Rnase-free	4.80 (± 0.01)	POS	NEG	NEG	NEG	NEG
	Aquafina	Demineralized water, reverse osmosis	5.05 (± 0.01)	POS	NEG	NEG	NEG	NEG
	S. Pellegrino	Carbonated natural mineral water	5.09 (± 0.01)	POS	NEG	NEG	NEG	NEG
	Canadian Springs	Distilled water, osonized	5.31 (± 0.01)	POS	NEG	NEG	NEG	NEG
	Dasani	Remineralized water, reverse osmosis treated	5.68 (± 0.01)	POS	NEG	NEG	NEG	NEG
	Big8	Distilled water, ozonated	6.25 (± 0.01)	POS	NEG	NEG	NEG	NEG
	Big8	Spring water, ozonated	6.26 (± 0.01)	POS	NEG	NEG	NEG	NEG
	Glaceau Smart	Vapour distilled water with added electrolytes	6.71 (± 0.02)	POS	NEG	NEG	NEG	NEG
	N/A	Municipal water (Halifax, Nova Scotia, May12, 2021)	6.75 (± 0.02)	POS	NEG	NEG	NEG	NEG
	Fiji	Natural spring water, tropical rain filtered through volcanic rock	7.25 (± 0.02)	POS	NEG	NEG	NEG	NEG
	Simple Drop	Natural spring water	7.26 (± 0.02)	POS	NEG	NEG	NEG	NEG
	Pathwater	Purified water, reverse osmosis treated,	7.27 (± 0.01)	POS	NEG	NEG	NEG	NEG

medRxiv preprint doi: https://doi.org/10.1101/2021.07.04.21259490; this version posted July 6, 2021. The copyright holder for this preprint (which was not certified by peer review) is the author/funder, who has granted medRxiv a license to display the preprint in perpetuity. All rights reserved. No reuse allowed without permission.

		ozonated, and electrolytes added, pH-balanced, pH 7.5+						
	Art Life WTR	Purified water, mineralized and electrolytes added, pH-balanced	7.28 (± 0.01)	POS	NEG	NEG	NEG	NEG
	Evian	Spring water, natural electrolytes, pH 7.2	7.39 (± 0.02)	POS	NEG	NEG	NEG	NEG
	N/A	Rain water (Halifax, Nova Scotia, May 12, 2021)	7.47 (± 0.01)	POS	NEG	NEG	NEG	NEG
	Icelandic Glacial	Natural spring water	7.58 (± 0.02)	POS	NEG	NEG	NEG	NEG
	Nestle Pure Life	Natural spring water, ozonated	7.75 (± 0.02)	POS	NEG	NEG	NEG	NEG
	Earth Group	Spring water	7.80 (± 0.03)	POS	NEG	NEG	NEG	NEG
	Eska	Natural spring water, pH 7.4	7.81 (± 0.00)	POS	NEG	NEG	NEG	NEG
	#Smart Moodwater	Naturally alkaline spring water, pH 8+	7.91 (± 0.01)	POS	NEG	NEG	NEG	NEG
	Flow	Naturally alkaline spring water, pH 8.1	8.02 (± 0.00)	POS	NEG	NEG	NEG	NEG
	Glaceau Smart	Mineralized treated water, alkaline pH 9+	9.33 (± 0.00)	POS	NEG	NEG	NEG	NEG
Laboratory buffers and media (n=14)	Teligent	0.9% Saline	5.62 (± 0.02)	POS (weak)	NEG	NEG	NEG	NEG
	Boston BioProducts	0.5M Pipes buffer, pH 6.8	6.66 (± 0.01)	POS*	NEG	NEG	NEG	NEG
	FisherScientific	10 mM Tris-HCl; 1 mM EDTA (TE) buffer, molecular-	7.14 (± 0.01)	POS	NEG	NEG	NEG	NEG

medRxiv preprint doi: https://doi.org/10.1101/2021.07.04.21259490; this version posted July 6, 2021. The copyright holder for this preprint (which was not certified by peer review) is the author/funder, who has granted medRxiv a license to display the preprint in perpetuity. All rights reserved. No reuse allowed without permission.

		grade pH 7.4						
	Sigma Life Sciences	Dulbecco's Phosphate Buffered Saline (PBS)	7.18 (± 0.01)	POS*	NEG	NEG	NEG	NEG
	LiofilChem	Viral Transport Media (VTM)	7.24 (± 0.01)	POS*	NEG	NEG	NEG	NEG
	Redoxica	Viral Transport Media (VTM) with fetal bovine serum (FBS)	7.33 (± 0.01)	POS*	NEG	NEG	NEG	NEG
	Becton Dickinson	Veritor sample buffer	7.33 (± 0.00)	NEG	NEG	NEG	NEG	NEG
	Copan Diagnostics	Universal Transport Medium (UTM)	7.37 (± 0.01)	NEG	NEG	NEG	NEG	NEG
	Yokon	Universal Transport Medium (UTM)	7.44 (± 0.01)	NEG	NEG	NEG	NEG	NEG
	Gibco	RPMI medium 1640, with HEPES	7.48 (± 0.01)	NEG	NEG	NEG	NEG	NEG
	Genesis	KaiBiLi Extended ViralTrans, includes HEPES	7.50 (± 0.01)	NEG	NEG	NEG	NEG	NEG
	Gibco	Minimal Essential Media (MEM)	7.83 (± 0.01)	NEG	NEG	NEG	NEG	NEG
	Gibco	1x Phosphate Buffered Saline (PBS), pH 7.4	8.20 (± 0.01)	NEG	NEG	NEG	NEG	NEG
	Abbott	Panbio sample buffer	8.78 (± 0.01)	NEG	NEG	NEG	NEG	NEG
Clinical specimens (n=120)	N/A	NP swabs in UTM (n=30)	N/A	POS* (28/30)	NEG	NEG	NEG	NEG
	N/A	OP/N swabs in PBS (n=30)	N/A	POS* (26/30)	NEG	NEG	NEG	NEG
	N/A	BALs (n=30)	N/A	POS* (27/30)	NEG	NEG	NEG	NEG

medRxiv preprint doi: https://doi.org/10.1101/2021.07.04.21259490; this version posted July 6, 2021. The copyright holder for this preprint (which was not certified by peer review) is the author/funder, who has granted medRxiv a license to display the preprint in perpetuity. All rights reserved. No reuse allowed without permission.

	N/A	Saline gargles (n=30)	N/A	POS* (27/30)	NEG	NEG	NEG	NEG

*Only weak positive reactions were observed.

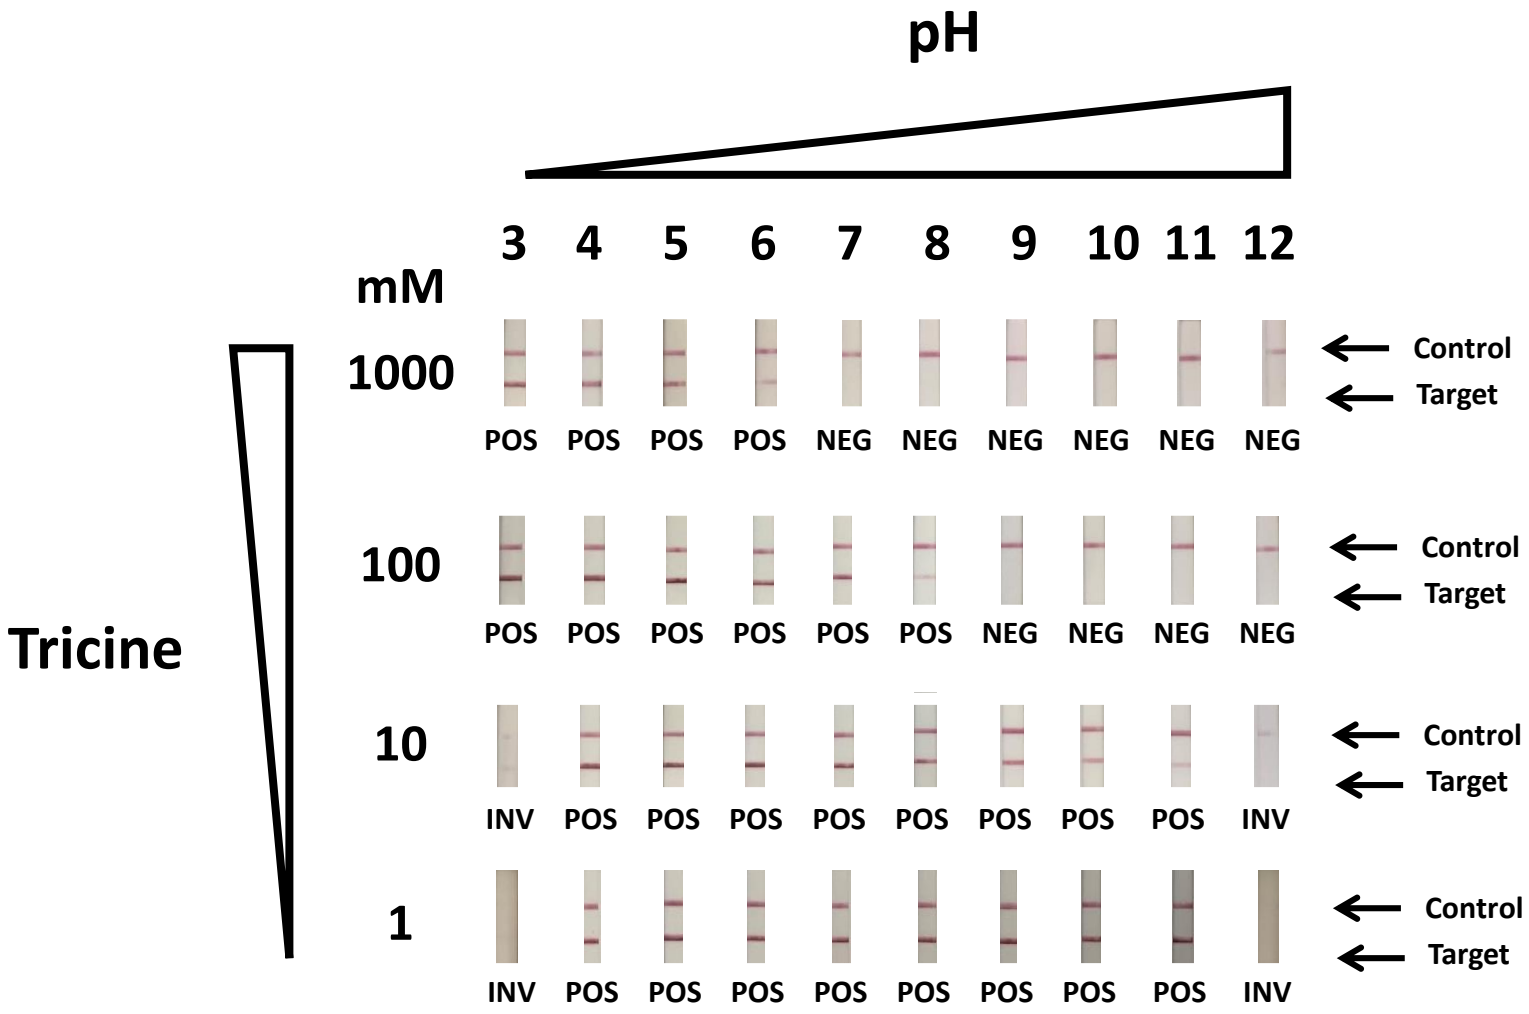
pH
3 4 5 6 7 8 9 10 11 12
mM
Tricine
1000
POS POS POS POS NEG NEG NEG NEG NEG NEG
100
POS POS POS POS POS POS NEG NEG NEG NEG
10
INV POS POS POS POS POS POS POS POS INV
1
INV POS POS POS POS POS POS POS POS INV
Control
Target

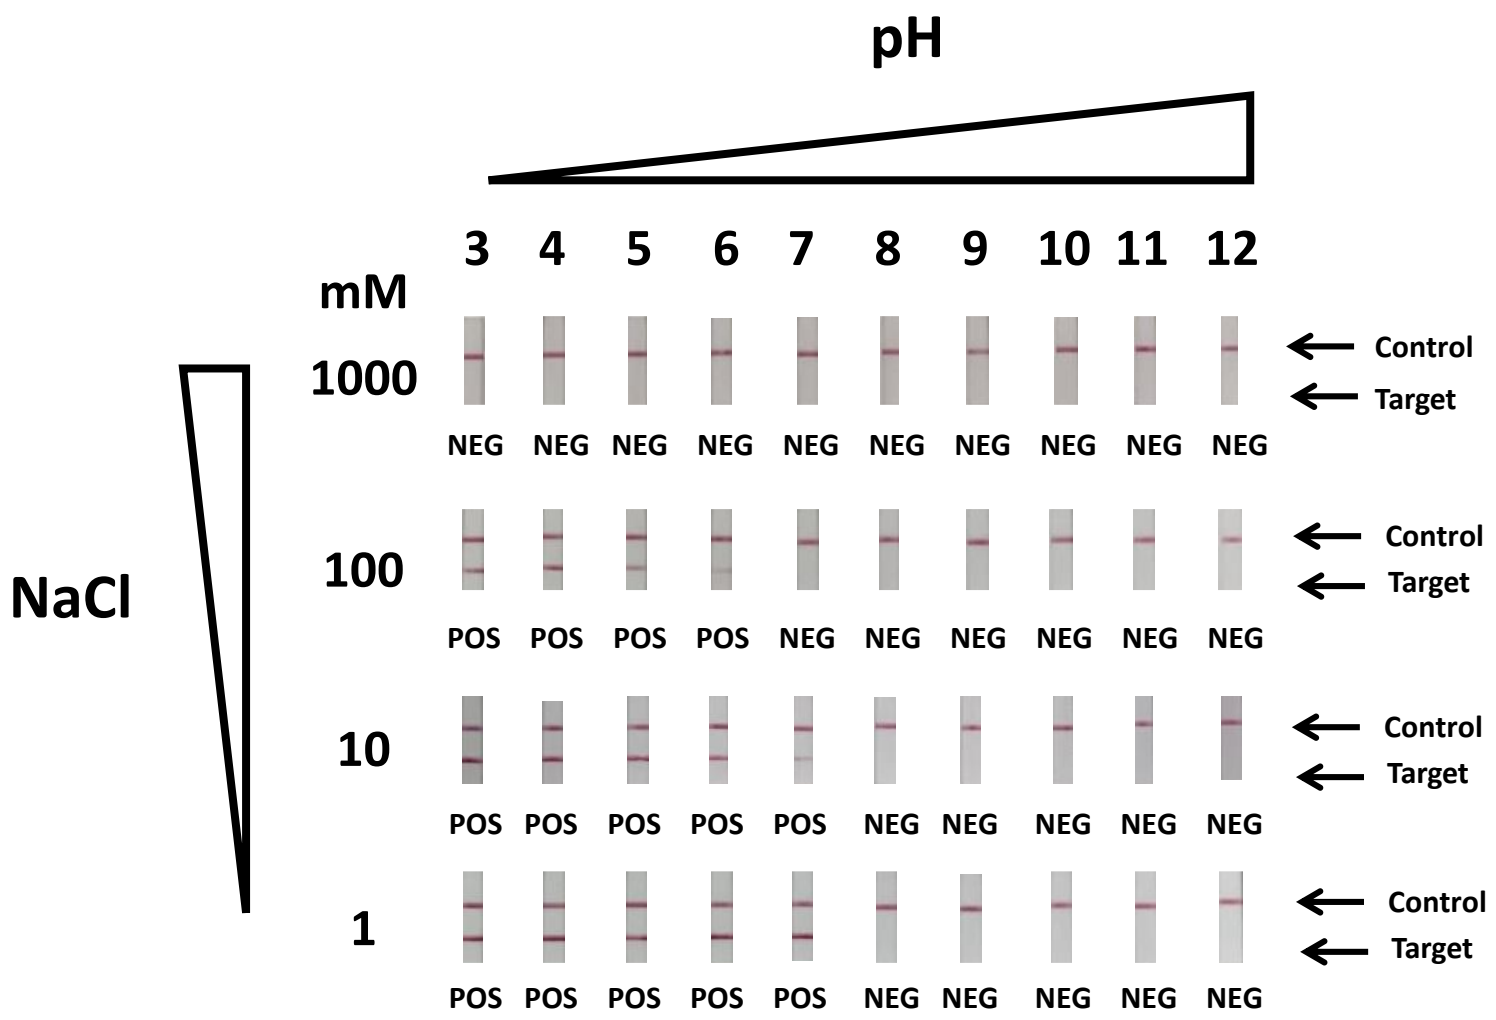
pH
3 4 5 6 7 8 9 10 11 12
mM
NaCl
1000
NEG NEG NEG NEG NEG NEG NEG NEG NEG NEG
100
POS POS POS POS NEG NEG NEG NEG NEG NEG
10
POS POS POS POS POS NEG NEG NEG NEG NEG
1
POS POS POS POS POS NEG NEG NEG NEG NEG
Control
Target

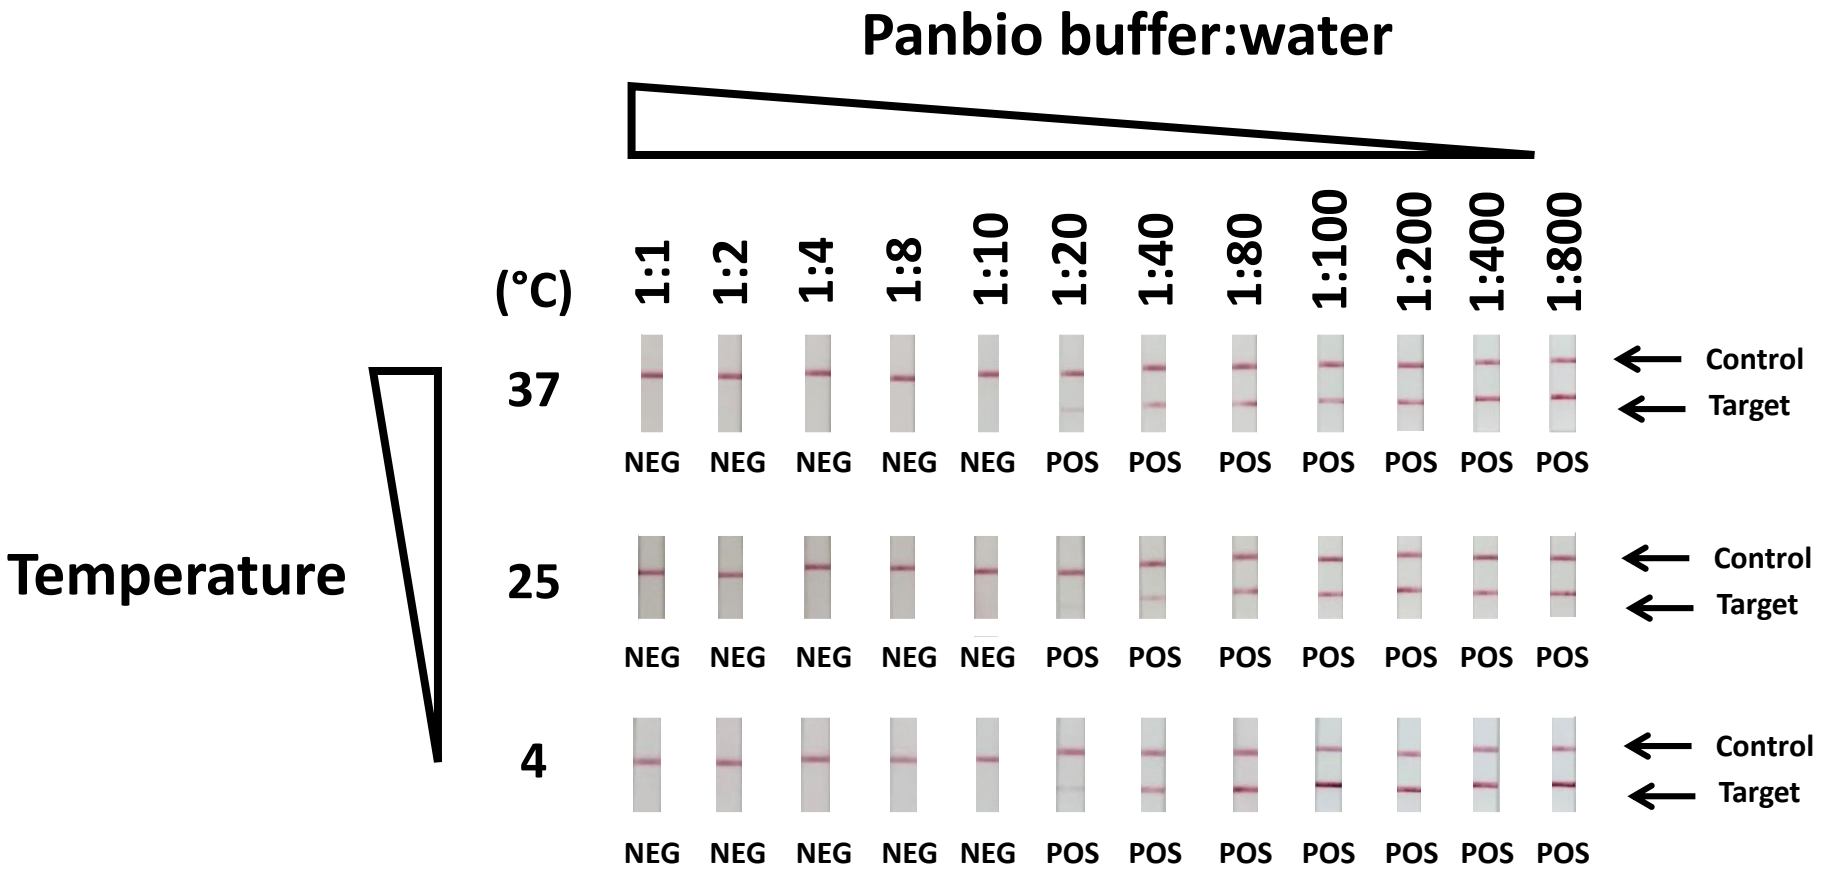
Panbio buffer:water
(°C)
1:1
1:2
1:4
1:8
1:10
1:20
1:40
1:80
1:100
1:200
1:400
1:800
Temperature
37
NEG NEG NEG NEG NEG POS POS POS POS POS POS POS
Control
Target
25
NEG NEG NEG NEG NEG POS POS POS POS POS POS POS
Control
Target
4
NEG NEG NEG NEG NEG POS POS POS POS POS POS POS
Control
Target