medRxiv preprint doi: https://doi.org/10.1101/2021.07.26.21261162; this version posted July 30, 2021. The copyright holder for this preprint (which was not certified by peer review) is the author/funder, who has granted medRxiv a license to display the preprint in perpetuity. It is made available under a CC-BY-ND 4.0 International license .

Diagnostic performance of a novel digital immunoassay (RapidTesta SARS-CoV-2): a prospective observational study with 1,127 nasopharyngeal samples

Hiromichi Suzuki[a,b,e*], Yusaku Akashi[b,c], Atsuo Ueda[d], Yoshihiko Kiyasu[b,e], Yuto Takeuchi[b,e], Yuta Maehara[f], Yasushi Ochiai[f], Shinya Okuyama[f], Shigeyuki Notake[d], Koji Nakamura[d], Hiroichi Ishikawa[h]

[a]Department of Infectious Diseases, Faculty of Medicine, University of Tsukuba, 1-1-1 Tennodai, Tsukuba, Ibaraki 305-8575, Japan

[b]Division of Infectious Diseases, Department of Medicine, Tsukuba Medical Center Hospital, 1-3-1 Amakubo Tsukuba, Ibaraki 305-8558, Japan

[c]Akashi Internal Medicine Clinic, 3-1-63 Asahigaoka, Kashiwara, Osaka 582-0026, Japan

[d]Department of Clinical Laboratory, Tsukuba Medical Center Hospital, 1-3-1 Amakubo, Tsukuba, Ibaraki 305-8558, Japan

[e]Department of Infectious Diseases, University of Tsukuba Hospital, 2-1-1 Amakubo,

NOTE: This preprint reports new research that has not been certified by peer review and should not be used to guide clinical practice.

medRxiv preprint doi: https://doi.org/10.1101/2021.07.26.21261162; this version posted July 30, 2021. The copyright holder for this preprint (which was not certified by peer review) is the author/funder, who has granted medRxiv a license to display the preprint in perpetuity. It is made available under a CC-BY-ND 4.0 International license .

Tsukuba, Ibaraki 305-8576, Japan

[f]Sekisui Medical Co., Ltd. Research & Development Division, Urban Net Nihonbashi 2-chome Building, 2-1-3 Nihonbashi, Chuo-ku, Tokyo 103-0027, Japan

[g]Department of Respiratory Medicine, Tsukuba Medical Center Hospital, 1-3-1 Amakubo Tsukuba, Ibaraki 305-8558, Japan

[h]Department of Respiratory Medicine, Tsukuba Medical Center Hospital, 1-3-1 Amakubo Tsukuba, Ibaraki 305-8558, Japan

E-mail addresses of each author: Hiromichi Suzuki, hsuzuki@md.tsukuba.ac.jp; Yusaku Akashi, yusaku-akashi@umin.ac.jp; Atsuo Ueda, atsuo.ueda06090727@outlook.jp; Yoshihiko Kiyasu, kiyasu-tuk@umin.ac.jp; Yuto Takeuchi, yuto-takeuchi@umin.ac.jp; Yuta Maehara, yuta.maehara@sekisui.com; Yasushi Ochiai, yasushi-ochiai@sekisui.com; Shinya Okuyama, shinya.okuyama@sekisui.com; Shigeyuki Notake, notake@tmch.or.jp; Koji Nakamura, koji-nakamura@tmch.or.jp; Hiroichi Ishikawa, hishikawa@tmch.or.jp

medRxiv preprint doi: https://doi.org/10.1101/2021.07.26.21261162; this version posted July 30, 2021. The copyright holder for this preprint (which was not certified by peer review) is the author/funder, who has granted medRxiv a license to display the preprint in perpetuity. It is made available under a CC-BY-ND 4.0 International license .

* Correspondence to:

Hiromichi Suzuki, MD, PhD

Professor, Department of Infectious Diseases, Faculty of Medicine, University of Tsukuba, 1-1-1 Tennodai, Tsukuba, Ibaraki, 305-8575, Japan

Tel: +81-29-853-3210

E-mail: hsuzuki@md.tsukuba.ac.jp

Authorship statement.

All authors meet the ICMJE authorship criteria.

Contributors: All authors performed the investigation. Hiromichi Suzuki supervised the project and drafted the manuscript. All authors contributed to the writing of the final manuscript.

medRxiv preprint doi: https://doi.org/10.1101/2021.07.26.21261162; this version posted July 30, 2021. The copyright holder for this preprint (which was not certified by peer review) is the author/funder, who has granted medRxiv a license to display the preprint in perpetuity. It is made available under a CC-BY-ND 4.0 International license .

Abstract

Introduction: Digital immunoassays are generally regarded as superior tests for the detection of infectious disease pathogens, but there have been insufficient data concerning SARS-CoV-2 immunoassays.

Methods: We prospectively evaluated a novel digital immunoassay (RapidTesta SARS-CoV-2). Two nasopharyngeal samples were simultaneously collected for antigen tests and RT-PCR. Real-time RT-PCR for SARS-CoV-2, using a method developed by the National Institute of Infectious Diseases, Japan, served as the reference RT-PCR method.

Results: During the study period, 1,127 nasopharyngeal samples (symptomatic patients: 802, asymptomatic patients: 325) were evaluated. For digital immunoassay antigen tests, the sensitivity was 78.3% (95% CI: 67.3%–87.1%) and the specificity was 97.6% (95% CI: 96.5%–98.5%). When technicians visually analyzed the antigen test results, the sensitivity was 71.6% (95% CI: 59.9%–81.5%) and the specificity was 99.2% (95% CI: 98.5%–99.7%). Among symptomatic patients, the sensitivity was 89.4% (95% CI; 76.9%–96.5%) with digital immunoassay antigen tests, and 85.1%

medRxiv preprint doi: https://doi.org/10.1101/2021.07.26.21261162; this version posted July 30, 2021. The copyright holder for this preprint (which was not certified by peer review) is the author/funder, who has granted medRxiv a license to display the preprint in perpetuity. It is made available under a CC-BY-ND 4.0 International license .

(95% CI; 71.7%–93.8%) with visually analyzed the antigen test, respectively.

Conclusions: The findings indicated that RapidTesta SARS-CoV-2 analysis with the DIA device had sufficient analytical performance for the detection of SARS-CoV-2 in nasopharyngeal samples. When positive DIA results are recorded without a visually recognizable red line at the positive line location on the test cassette, additional RT-PCR evaluation should be performed.

Keywords: RapidTesta SARS-CoV-2, digital immunoassay, nasopharyngeal sample, SARS-CoV-2, COVID-19, asymptomatic patients

medRxiv preprint doi: https://doi.org/10.1101/2021.07.26.21261162; this version posted July 30, 2021. The copyright holder for this preprint (which was not certified by peer review) is the author/funder, who has granted medRxiv a license to display the preprint in perpetuity. It is made available under a CC-BY-ND 4.0 International license .

Introduction

COVID-19 has been the primary global health concern for 2 consecutive years (2020 and 2021) and its diagnosis has been mainly performed by respiratory sampling [1]. RT-PCR has been regarded as the "gold standard" method [1] for the detection of SARS-CoV-2, but a long turnaround time is needed for evaluation of the results.

Immunochromatographic antigen testing is a widely used laboratory technique for the detection of SARS-CoV-2 owing to its ease of handling and rapid acquisition of results [2, 3]; moreover, a strong correlation between antigen test results and SARS-CoV-2 infectivity has been reported [4]. In recent years, improved sensitivities for pathogen detection using digital immunoassay devices have been proven, especially in the field of influenza [5], and applications to COVID-19 diagnosis have been expected.

The RapidTesta SARS-CoV-2 is a novel immunochromatographic assay that can detect SARS-CoV-2 in 10 minutes; it was newly approved in Japan in June 2021. The RapidTesta SARS-CoV-2 can be analyzed using a portal digital immunoassay (DIA) device, with presumably greater sensitivity compared with human-eye judgment.

Herein, we performed a prospective comparison with a DIA device and RT-PCR using

medRxiv preprint doi: https://doi.org/10.1101/2021.07.26.21261162; this version posted July 30, 2021. The copyright holder for this preprint (which was not certified by peer review) is the author/funder, who has granted medRxiv a license to display the preprint in perpetuity. It is made available under a CC-BY-ND 4.0 International license .

a set of two simultaneously collected nasopharyngeal samples from multiple patients.

Patients and Methods

The current study was prospectively performed between April 20, 2021, and May 31, 2021, at a "drive-through" PCR center in Tsukuba Medical Center Hospital (TMCH), Tsukuba, Japan. During the study period, patients were mainly referred from 63 clinic and a local public health center. Informed consent was obtained from all participating patients and the study was performed with the approval of the TMCH ethical committee (approval number: 2021-021).

Study process and evaluation of antigen test results with and without the use of a digital immunoassay device

In this study, two nasopharyngeal samples were simultaneously collected with FLOQ Swabs (Copan Italia S.p.A., Brescia, Italy) for RT-PCR and flocked type swabs (contained in the RapidTesta SARS-CoV-2 kit) for antigen tests, as previously described [6]. For antigen tests, each swab was diluted into extraction buffer; three drops of the

medRxiv preprint doi: https://doi.org/10.1101/2021.07.26.21261162; this version posted July 30, 2021. The copyright holder for this preprint (which was not certified by peer review) is the author/funder, who has granted medRxiv a license to display the preprint in perpetuity. It is made available under a CC-BY-ND 4.0 International license .

extracted sample were then added to a test cassette through filtration (Figure 1). The examination time was 10 minutes; the analysis was performed both visually and automatically with a DIA device (Figure 2).

For RT-PCR, each swab was diluted in 3 mL of Universal Transport Medium (BD), then transferred to the microbiology department of the TMCH for RNA extraction and in-house RT-PCR. Extraction was performed with magLEAD 6gC (Precision System Science Co., Ltd., Chiba, Japan) with a 200µL aliquot of each nasopharyngeal sample. In total, 100 µL of purified sample were eluted and subjected to in-house RT-PCR analysis [7] and a reference real-time RT-PCR analysis for SARS-CoV-2, which used a method developed by the National Institute of Infectious Diseases, Japan (NIID method) [8]. The reference RT-PCR analysis was performed at Tsukuba Research Institute of Sekisui Medical Co., Ltd.; eluted samples were transported weekly for evaluation. Before evaluation, all samples were preserved at –80°C.

Reference RT-PCR using a method developed by the National Institute of Infectious Diseases, Japan

medRxiv preprint doi: https://doi.org/10.1101/2021.07.26.21261162; this version posted July 30, 2021. The copyright holder for this preprint (which was not certified by peer review) is the author/funder, who has granted medRxiv a license to display the preprint in perpetuity. It is made available under a CC-BY-ND 4.0 International license .

The NIID method has been regarded as the "gold standard" RT-PCR method for SARS-CoV-2 detection and was used as the reference RT-PCR method in this study. The NIID method was performed with duplicate N and N2 assay analysis, as previous described [8]. The CFX96 Touch Real-Time PCR Detection System (Bio-Rad Laboratories, Hercules, CA, USA) and Reliance One-Step Multiplex Supermix (Bio-Rad Laboratories) were used for analysis. In the event of discordance between the reference RT-PCR and in-house RT-PCR results, the GeneXpert® system and an Xpert® Xpress SARS-CoV-2 assay (Cepheid Inc., Sunnyvale, CA, USA) [9] were used for additional evaluation.

Statistical analysis

The sensitivity, specificity, positive predictive value, and negative predictive value of antigen test results were calculated using the Clopper and Pearson method, with 95% confidence intervals (CIs). All calculations were conducted using R software, version 4.1.0 (www.r-project.org).

medRxiv preprint doi: https://doi.org/10.1101/2021.07.26.21261162; this version posted July 30, 2021. The copyright holder for this preprint (which was not certified by peer review) is the author/funder, who has granted medRxiv a license to display the preprint in perpetuity. It is made available under a CC-BY-ND 4.0 International license .

Results

During the study period, 1,127 nasopharyngeal samples were collected for evaluation. In total, 802 samples were collected from symptomatic patients and 325 samples were collected from asymptomatic patients.

Of the 1,127 samples, 74 (6.6%) were positive according to RT-PCR with the NIID method. There were no instances of discordance between RT-PCR with the NIID method and in-house RT-PCR; thus, no additional evaluations with the GeneXpert® system were performed.

The results of the RapidTesta SARS-CoV-2 without the use of a DIA device are shown in Table 1-a. The sensitivity was 71.6% (95% CI: 59.9%–81.5%), and the specificity was 99.2% (95% CI: 98.5%–99.7%). The positive predictive value was 86.9% (95% CI: 75.8%–94.2%), and the negative predictive value was 98.0% (95% CI: 97.0%–98.8%).

The results of the RapidTesta SARS-CoV-2 with the use of a DIA device are shown in Table 1-b. The sensitivity was 78.4% (95% CI: 67.3%–87.1%), and the specificity was 97.6% (95% CI: 96.5%–98.5%). The positive predictive value was 69.9% (95% CI: 58.8%–79.5%), and the negative predictive value was 98.5% (95% CI: 97.5%–99.1%).

medRxiv preprint doi: https://doi.org/10.1101/2021.07.26.21261162; this version posted July 30, 2021. The copyright holder for this preprint (which was not certified by peer review) is the author/funder, who has granted medRxiv a license to display the preprint in perpetuity. It is made available under a CC-BY-ND 4.0 International license .

The results of the RapidTesta SARS-CoV-2 with/without the use of a DIA device are shown in Table 2-a and Table 2-b. For the RapidTesta SARS-CoV-2 without the use of a DIA device, the sensitivity was 85.1% (95% CI: 71.7%–93.8%), and the specificity was 99.3% (95% CI: 98.5%–99.8%). For the RapidTesta SARS-CoV-2 with the use of a DIA device, the sensitivity was 89.4% (95% CI: 76.9%–96.5%), and the specificity was 97.7% (95% CI: 96.4%–98.7%).

The sensitivities stratified according to Ct value are shown in Table 3. Without the use of a DIA device (Table 3-a), the sensitivity for Ct < 20 was 96.4% (95% CI: 81.7%–99.9%); the sensitivity was 81.3% (95% CI: 63.6%–92.8%) for Ct 20–29. No positive samples (Ct ≥ 30) were detected without the use of a DIA device. When using a DIA device (Table 3-b), the sensitivity for Ct < 20 was 100.0% (95% CI: 87.7%–100%); the sensitivities were 84.4% (95% CI: 67.2%–94.7%) for Ct 20–29 and 21.4% (95% CI: 4.7%–50.8%) for (Ct ≥ 30), respectively.

Discussion

This prospective study revealed that the sensitivity of the RapidTesta SARS-CoV-2

medRxiv preprint doi: https://doi.org/10.1101/2021.07.26.21261162; this version posted July 30, 2021. The copyright holder for this preprint (which was not certified by peer review) is the author/funder, who has granted medRxiv a license to display the preprint in perpetuity. It is made available under a CC-BY-ND 4.0 International license .

was 78.4% and the specificity was 97.6%. For symptomatic patients, the sensitivities were 85.1% for antigen tests without the use of a DIA device and 89.4% for antigen tests with the use of a DIA device. The sensitivity of DIA tests was superior to the sensitivity of visually analyzed antigen tests, but the rate of false-positive results increased with introduction of a DIA device.

A recent systematic review described overall antigen test sensitivities of 72.0% (95% CI: 63.7%–79.0%) for symptomatic patients and 58.1% (95% CI: 40.2%–74.1%) for asymptomatic patients [10]. For quantitative antigen tests, the overall sensitivity and specificity were 84.8% and 97.9%, respectively [11]. In the current study, the sensitivity for symptomatic patients of RapidTesta SARS-CoV-2 was over 80% and it is considered to meet the acceptable criteria of antigen test recommended by the World Health Organization[12].

To our knowledge, there have been few evaluations of DIA devices for the detection of SARS-CoV-2. Most recently, a prospective study of a DIA device (QuickChaser Auto SARS-CoV-2) with 1,401 nasopharyngeal samples showed that the sensitivity and specificity were 74.7% (95% CI: 64.0%–83.6%) and 99.8% (95% CI: 99.5%–100%),

medRxiv preprint doi: https://doi.org/10.1101/2021.07.26.21261162; this version posted July 30, 2021. The copyright holder for this preprint (which was not certified by peer review) is the author/funder, who has granted medRxiv a license to display the preprint in perpetuity. It is made available under a CC-BY-ND 4.0 International license .

respectively [13]. The sensitivity for positive samples (Ct < 30) was 98.2% (56/57). In our study, the overall sensitivity of the RapidTesta SARS-CoV-2 with a DIA device was comparable with a previous DIA device (QuickChaser Auto SARS-CoV-2). This rapid analysis could be completed within 10 minutes, although its sensitivity for positive samples (Ct < 30) (91.7%; 55/60) was slightly inferior to the previously described DIA device.

False-positive results that indicate the presence of COVID-19 cause substantial harm in clinical practice [14] and the emergence of false-positive results has been repeatedly reported in Japan [15-17]. In the current study, the increased sensitivity when using the DIA device was negatively associated with the decrease of specificity. False-positive results were frequently observed (17/25; 68.0%) via DIA inspection for samples with RT-PCR-negative results in this study. The current study suggested that additional SARS-CoV-2 evaluation should be performed when positive RapidTesta SARS-CoV-2 results with a DIA device are recorded in the absence of a visually recognizable positive line.

There were some limitations to this study. First, study samples were collected in a

medRxiv preprint doi: https://doi.org/10.1101/2021.07.26.21261162; this version posted July 30, 2021. The copyright holder for this preprint (which was not certified by peer review) is the author/funder, who has granted medRxiv a license to display the preprint in perpetuity. It is made available under a CC-BY-ND 4.0 International license .

local district in Japan in the spring of 2021. Second, differences among variant strains were not analyzed. Third, study samples were collected from the nasopharyngeal tract and saliva samples were not analyzed. Fourth, improvements of DIA specificity were not examined and further investigations are necessary.

In conclusion, this study showed that the RapidTesta SARS-CoV-2 with a DIA device had sufficient analytical performance for the detection of SARS-CoV-2 in nasopharyngeal samples. When positive DIA results are recorded without a visually recognizable red line at the positive line location on the test cassette, additional RT-PCR evaluation should be performed.

Acknowledgements

We thank Mrs. Yoko Ueda, Mrs. Mio Matsumoto, Mr. Masaomi Matsubayashi, Mrs. Mika Yaguchi, Mrs. Yumiko Tanaka, and the staff of the Department of Clinical Laboratory of Tsukuba Medical Center Hospital for their support of this study. We thank all participating medical institutions for providing their patients' clinical information. Mrs. Yoko Ueda and Mrs. Mio Matsumoto substantially contributed to creating the

medRxiv preprint doi: https://doi.org/10.1101/2021.07.26.21261162; this version posted July 30, 2021. The copyright holder for this preprint (which was not certified by peer review) is the author/funder, who has granted medRxiv a license to display the preprint in perpetuity. It is made available under a CC-BY-ND 4.0 International license .

database for this study.

Conflict of Interest

Sekisui Medical Co., Ltd. provided fees for research expenses and provided the RapidTesta SARS-CoV-2 without charge. Yuta Maehara, Yasushi Ochiai, and Shinya Okuyama belong to Sekisui Medical Co., Ltd., the developer of the RapidTesta SARS-CoV-2.

medRxiv preprint doi: https://doi.org/10.1101/2021.07.26.21261162; this version posted July 30, 2021. The copyright holder for this preprint (which was not certified by peer review) is the author/funder, who has granted medRxiv a license to display the preprint in perpetuity. It is made available under a CC-BY-ND 4.0 International license .

References

[1] World Health Organization. Coronavirus disease (COVID-19) Weekly Epidemiological Update and Weekly Operational Update. https://www.who.int/emergencies/diseases/novel-coronavirus-2019/situation-reports [accessed July 10, 2021].

[2] Safiabadi Tali SH, LeBlanc JJ, Sadiq Z, Oyewunmi OD, Camargo C, Nikpour B, et al. Tools and techniques for severe acute respiratory syndrome coronavirus 2 (SARS-CoV-2)/COVID-19 detection. Clin Microbiol Rev. 2021;34. e00228-20

[3] Hanson KE, Altayar O, Caliendo AM, Arias CA, Englund JA, Hayden MK, et al. The Infectious Diseases Society of America Guidelines on the Diagnosis of COVID-19: Antigen Testing. Clin Infect Dis. 2021. (Ahead of print)

[4] Korenkov M, Poopalasingam N, Madler M, Vanshylla K, Eggeling R, Wirtz M, et al. Evaluation of a rapid antigen test to detect SARS-CoV-2 infection and identify potentially infectious

medRxiv preprint doi: https://doi.org/10.1101/2021.07.26.21261162; this version posted July 30, 2021. The copyright holder for this preprint (which was not certified by peer review) is the author/funder, who has granted medRxiv a license to display the preprint in perpetuity. It is made available under a CC-BY-ND 4.0 International license .

individuals. J Clin Microbiol. 2021. (Ahead of print)

[5] Merckx J, Wali R, Schiller I, Caya C, Gore GC, Chartrand C, et al. Diagnostic accuracy of novel and traditional rapid tests for influenza infection compared with reverse transcriptase polymerase chain reaction: a systematic review and meta-analysis. Ann Intern Med. 2017;167:394–409.

[6] Marty FM, Chen K, Verrill KA. How to obtain a nasopharyngeal swab specimen. N Engl J Med. 2020;382:e76.

[7] Kiyasu Y, Akashi Y, Sugiyama A, Takeuchi Y, Notake S, Naito A, et al. A Prospective evaluation of the analytical performance of GENECUBE((R)) HQ SARS-CoV-2 and GENECUBE((R)) FLU A/B. Mol Diagn Ther. 2021;25:495–504.

[8] Shirato K, Nao N, Katano H, Takayama I, Saito S, Kato F, et al. Development of genetic diagnostic methods for detection for novel coronavirus 2019(nCoV-2019) in Japan. Jpn J Infect Dis. 2020;73:304–7.

[9] Lee J, Song JU. Diagnostic accuracy of the Cepheid Xpert Xpress and the Abbott ID NOW assay for rapid detection of SARS-CoV-2: a systematic review and meta-analysis. J Med

medRxiv preprint doi: https://doi.org/10.1101/2021.07.26.21261162; this version posted July 30, 2021. The copyright holder for this preprint (which was not certified by peer review) is the author/funder, who has granted medRxiv a license to display the preprint in perpetuity. It is made available under a CC-BY-ND 4.0 International license .

Virol. 2021;93:4523–31.

[10] Dinnes J, Deeks JJ, Berhane S, Taylor M, Adriano A, Davenport C, et al. Rapid, point-of-care antigen and molecular-based tests for diagnosis of SARS-CoV-2 infection. Cochrane Database Syst Rev. 2021;3:CD013705.

[11] Hirotsu Y, Sugiura H, Maejima M, Hayakawa M, Mochizuki H, Tsutsui T, et al. Comparison of Roche and Lumipulse quantitative SARS-CoV-2 antigen test performance using automated systems for the diagnosis of COVID-19. Int J Infect Dis. 2021;108:263–9.

[12] World Health Organization. COVID-19 Target product profiles for priority diagnostics to support response to the COVID-19 pandemic v.1.0 2020:1–38. https://www.who.int/publications/m/item/covid-19-target-product-profiles-for-priority-diagnostics-to-support-response-to-the-covid-19-pandemic-v.0.1 (accessed July 13, 2021)

[13] Kurihara Y, Kiyasu Y, Akashi Y, Takeuchi Y, Narahara K, Mori S, et al. The evaluation of a novel digital immunochromatographic assay with silver amplification to detect SARS-CoV-2. J Infect Chemother. (Ahead of print)

[14] Healy B, Khan A, Metezai H, Blyth I, Asad H. The impact of false positive COVID-19 results in an area of low prevalence. Clin Med (Lond). 2021;21:e54–6.

medRxiv preprint doi: https://doi.org/10.1101/2021.07.26.21261162; this version posted July 30, 2021. The copyright holder for this preprint (which was not certified by peer review) is the author/funder, who has granted medRxiv a license to display the preprint in perpetuity. It is made available under a CC-BY-ND 4.0 International license .

[15] Itoh K, Kawamitsu T, Osaka Y, Sato K, Suzuki Y, Kiriba C, et al. False positive results in severe acute respiratory coronavirus 2 (SARS-CoV-2) rapid antigen tests for inpatients. J Infect Chemother. 2021;27:1089–91.

[16] Otake S, Miyamoto S, Mori A, Iwamoto T, Kasai M. False-positive results in SARS-CoV-2 antigen test with rhinovirus-A infection. Pediatr Int. 2021 (Ahead of print)

[17] Yamaniha K, Kinjo T, Akamine M, Setoguchi M, Tateyama M, Fujita J. False-positive for SARS-CoV-2 antigen test in a man with acute HIV infection. J Infect Chemother. 2021;27:1112–4.

medRxiv preprint doi: https://doi.org/10.1101/2021.07.26.21261162; this version posted July 30, 2021. The copyright holder for this preprint (which was not certified by peer review) is the author/funder, who has granted medRxiv a license to display the preprint in perpetuity. It is made available under a CC-BY-ND 4.0 International license .

Table 1-a.

Sensitivity and specificity of the RapidTesta SARS-CoV-2 without the use of a digital immunoassay device among all patients in the study.

		real-time RT-PCR	
		Positive	Negative
Antigen test	Positive	53	8
	Negative	21	1045
Sensitivity (%)		71.6(59.9-81.5)	
Specificity (%)		99.2(98.5-99.7)	

Reverse transcription-polymerase chain reaction findings were used as reference results.

RT-PCR, reverse transcription-polymerase chain reaction

Data in parentheses indicate 95% confidence intervals.

Table 1-b.

Sensitivity and specificity of the RapidTesta SARS-CoV-2 with the use of a digital immunoassay device among all patients in the study.

		real-time RT-PCR	
		Positive	Negative
Antigen test	Positive	58	25
	Negative	16	1028
Sensitivity (%)		78.4(67.3-87.1)	
Specificity (%)		97.6(96.5-98.5)	

Reverse transcription-polymerase chain reaction findings were used as reference results.

RT-PCR, reverse transcription-polymerase chain reaction

Data in parentheses indicate 95% confidence intervals.

medRxiv preprint doi: https://doi.org/10.1101/2021.07.26.21261162; this version posted July 30, 2021. The copyright holder for this preprint (which was not certified by peer review) is the author/funder, who has granted medRxiv a license to display the preprint in perpetuity. It is made available under a CC-BY-ND 4.0 International license .

Table 2-a.

Sensitivity and specificity of the RapidTesta SARS-CoV-2 without the use of a digital immunoassay device among symptomatic patients.

		real-time RT-PCR	
		Positive	Negative
Antigen test	Positive	40	5
	Negative	7	750
Sensitivity (%)		85.1(71.7-93.8)	
Specificity (%)		99.3(98.5-99.8)	

Table 2-b.

Sensitivity and specificity of the RapidTesta SARS-CoV-2 with the use of a digital immunoassay device among symptomatic patients.

		real-time RT-PCR	
		Positive	Negative
Antigen test	Positive	42	17
	Negative	5	738
Sensitivity (%)		89.4(76.9-96.5)	
Specificity (%)		97.7(96.4-98.7)	

medRxiv preprint doi: https://doi.org/10.1101/2021.07.26.21261162; this version posted July 30, 2021. The copyright holder for this preprint (which was not certified by peer review) is the author/funder, who has granted medRxiv a license to display the preprint in perpetuity. It is made available under a CC-BY-ND 4.0 International license .

Table 3-a.

Sensitivities of the RapidTesta SARS-CoV-2 without the use of a digital immunoassay device according to Ct value.

Ct value(N2)	Sensitivity (%)	Positive	Negative
<20	96.4(81.7-99.9)	27	1
20-29	81.3(59.0-91.7)	26	6
≥30	0(0-19.5)	0	14

Table 3-b.

Sensitivities of the RapidTesta SARS-CoV-2 with the use of a digital immunoassay device according to Ct value.

Ct value(N2)	Sensitivity (%)	Positive	Negative
<20	100(87.7-100)	28	0
20-29	84.4(63.1-93.9)	27	5
≥30	21.4(3.8-43.4)	3	11

medRxiv preprint doi: https://doi.org/10.1101/2021.07.26.21261162; this version posted July 30, 2021. The copyright holder for this preprint (which was not certified by peer review) is the author/funder, who has granted medRxiv a license to display the preprint in perpetuity. It is made available under a CC-BY-ND 4.0 International license .

Figure Legends

Figure 1. Test flow diagram of the RapidTesta SARS-CoV-2 without the use of a digital immunoassay device

Figure 2. Test flow diagram of the RapidTesta SARS-CoV-2 with the use of a digital immunoassay device

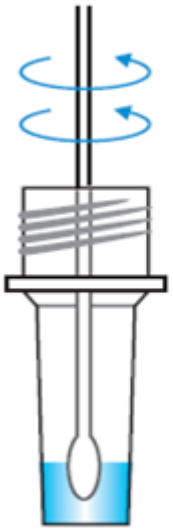

Extract swab sample into extraction buffer

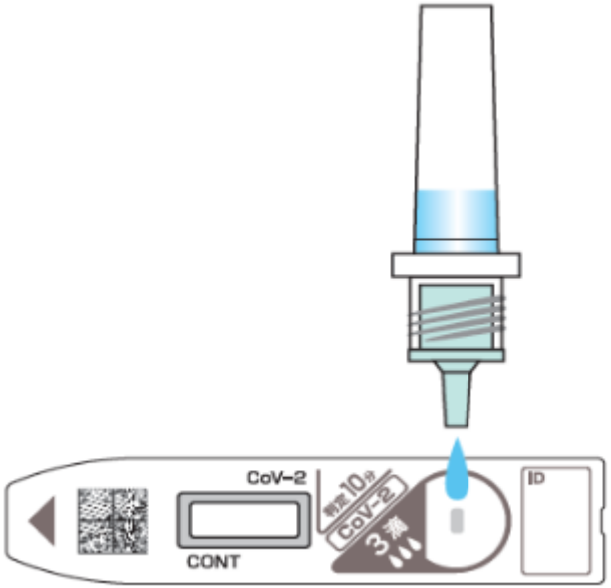

Add 3 drops of extracted sample onto the test cassette

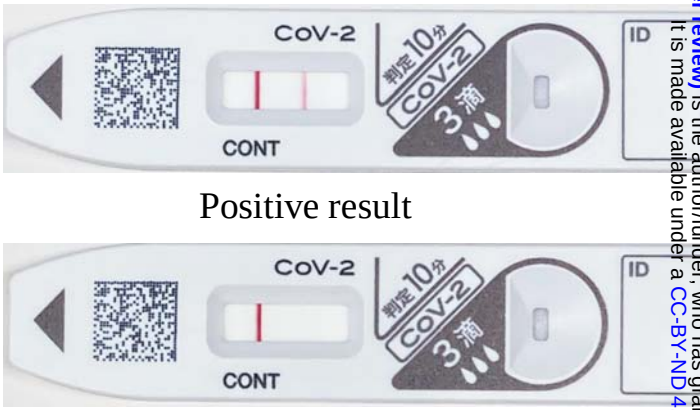

Positive result

Negative result

Judge the result by visual reading without using a digital immunoassay device

*Figures were edited from the Instruction for Use of RapidTesta SARS-CoV-2

medRxiv preprint doi: https://doi.org/10.1101/2021.07.26.21261162; this version posted July 30, 2021. The copyright holder for this preprint (which was not certified by peer review) is the author/funder, who has granted medRxiv a license to display the preprint in perpetuity. It is made available under a CC-BY-ND 4.0 International license.

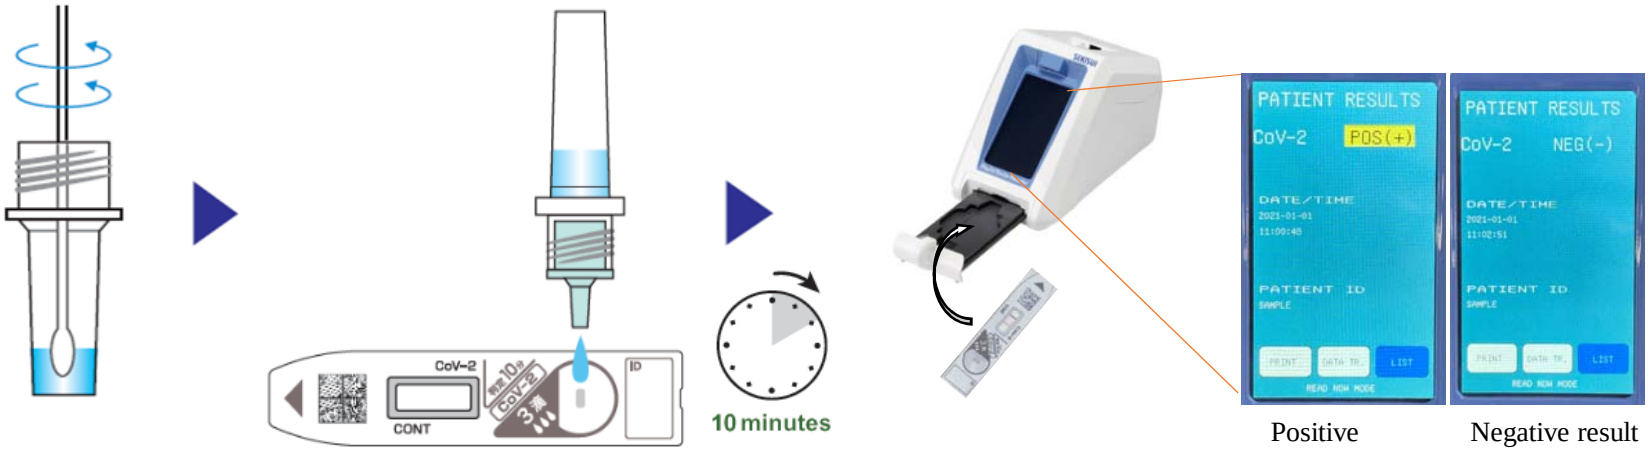

Extract swab sample into extraction buffer

Add 3 drops of extracted sample onto the test cassette

Positive result

Negative result

Judge the result by using a digital immunoassay device

*Figures were edited from the Instruction for Use of RapidTesta Reader

medRxiv preprint doi: https://doi.org/10.1101/2021.07.26.21261162; this version posted July 30, 2021. The copyright holder for this preprint (which was not certified by peer review) is the author/funder, who has granted medRxiv a license to display the preprint in perpetuity. It is made available under a CC-BY-ND 4.0 International license.