medRxiv preprint doi: https://doi.org/10.1101/2022.09.25.22280350; this version posted December 1, 2022. The copyright holder for this preprint (which was not certified by peer review) is the author/funder, who has granted medRxiv a license to display the preprint in perpetuity. All rights reserved. No reuse allowed without permission.

Thermal spread with Voyant 5 mm Fusion versus LigaSure 5 mm Blunt Tip Devices

Austin Carmack, MD[1+], Emma K. Satchell, MD[1*+], Apar S. Patel, MD[1+], Amir Bashiri, MD[1+], Burt Cagir, MD[1+], Anne Rizzo, MD[1+]

[1]Guthrie Robert Packer Hospital, Department of General Surgery, Sayre, PA, 18840, USA
*Corresponding author email: emma.satchell@guthrie.org
[+]These authors contributed equally to this work

WITHDRAWN
see manuscript DOI for details

ABSTRACT

Thermal spread is an unavoidable side-effect of electrocautery, however limiting it is important for minimizing damage to surrounding tissues. LigaSure 5 mm Blunt Tip has been in use since 2009 while Voyant 5 mm Fusion has only been FDA approved since 2018. Our hospital, a rural academic tertiary care center, recently moved to purchasing Voyant because of cost concerns. We aimed to compare the thermal spread of the two tools on raw pork meat at two different cut depths and on both right and left sides. The LigaSure device had significantly less thermal spread than Voyant across all measurements.

NOTE: This preprint reports new research that has not been certified by peer review and should not be used to guide clinical practice.

medRxiv preprint doi: https://doi.org/10.1101/2022.09.25.22280350; this version posted December 1, 2022. The copyright holder for this preprint (which was not certified by peer review) is the author/funder, who has granted medRxiv a license to display the preprint in perpetuity. All rights reserved. No reuse allowed without permission.

Introduction

A variety of surgical devices have been developed for electrocautery vessel sealing.(1) These tools are useful for decreasing operative time and lowering blood loss.(2) One of the downsides of these tools is the thermal spread that can damage surrounding structures.(3) LigaSure 5 mm Blunt Tip has been in use since 2009, while Voyant 5 mm Fusion has only been FDA approved for market sales since 2018.(4)

Thermal spread is an unavoidable side-effect of using electrocautery, however it damages surrounding tissues. Limiting thermal spread is an important goal of device manufacturers. Minimizing it is especially important when working with small vessels in tight spaces, such as in a thyroidectomy or esophagectomy.(5–7)

Our hospital, a rural academic tertiary care center, has recently moved to purchasing Voyant due to its lower cost. We aimed to compare the thermal spread of the tools at two different cut depths and on both right and left sides.

WITHDRAWN
See manuscript DOI for details

Methods

The data consisted of 224 measurements of thermal spread taken with digital caliper after activations from the Voyant 5 mm Fusion and LigaSure 5 mm Blunt Tip devices at cut-depths of 4mm and 8mm on the left and right sides on raw pork meat. This analysis compares the thermal spread of the two devices at the two sites (left and right), and the analysis is repeated for both cut-depths. A third analysis compares the sum of the thermal spread at the two sites by cut-depth.

In all three analyses the distribution of thermal spread is analyzed using two-way factorial analysis of variance (ANOVA). This approach tests whether there are significant differences between the thermal spreads by device and by side (left or right). It also tests for an interaction between the two, which would occur if the difference between devices was greater on one side compared to the other. The steps taken to conduct the ANOVA are (1) view the data graphically to determine evidence for device differences or an interaction, (2) conduct the statistical tests based on the ANOVA, and (3) if there is a significant interaction, determine which side shows the larger effect of the device.

Results

7mm Analysis

Figure 1 shows the distributions of thermal spread by side and device. The figure shows that the mean is greater on both sides for the Voyant device ($M_{\text{right}} = 2.54$, $M_{\text{left}} = 2.32$) than it is for the LigaSure device ($M_{\text{right}} = 1.58$, $M_{\text{left}} = 1.49$). In addition, the lines connecting the means for each side are roughly parallel. If an interaction were present, such that the devices differed more for one side than the other, these lines would not be parallel. No such evidence for an interaction is present in the figure.

Figure 1: Mean Thermal Spread by Device and Side

medRxiv preprint doi: https://doi.org/10.1101/2022.09.25.22280350; this version posted December 1, 2022. The copyright holder for this preprint (which was not certified by peer review) is the author/funder, who has granted medRxiv a license to display the preprint in perpetuity. All rights reserved. No reuse allowed without permission.

Figure 1:
Mean Thermal Spread by Device and Side

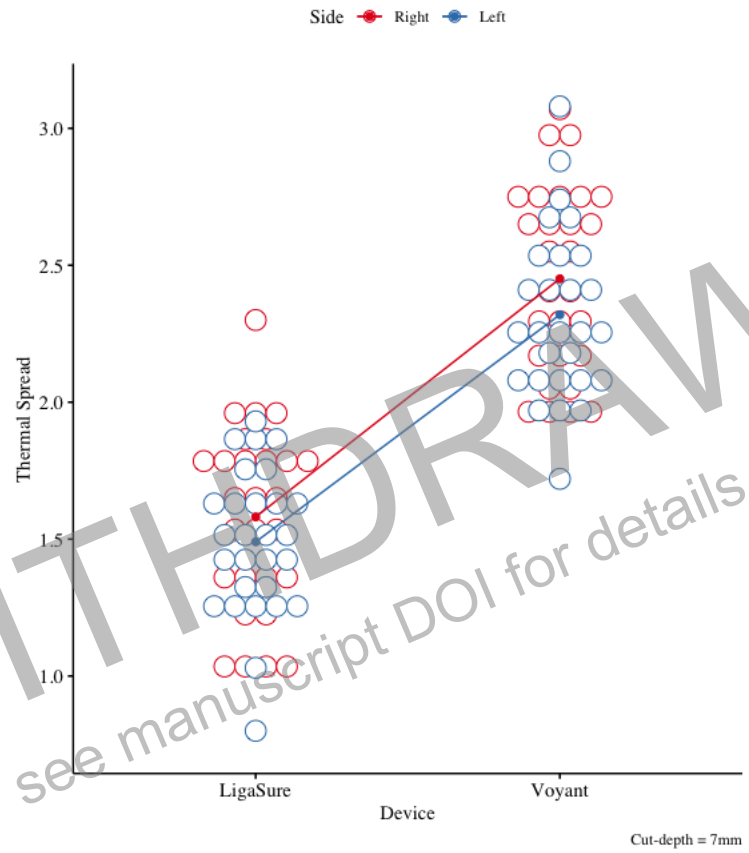

WITHDRAWN
see manuscript DOI for details

Table 1 gives the results of the two-way factorial ANOVA. The ANOVA confirms that that the interaction between side and device is not significant ( ). The main effect of device is statistically significant ($p < 0.001$), which indicates a significant difference in between the Voyant and LigaSure devices. The main effect of side is not significant ($p = 0.06$).

Table 1:
ANOVA Results (Cut-Depth: 7mm)

Term	SS: Type III	DF	F Statistic	P Value
Device	20.20	1	205.85	< 0.001
Side	0.35	1	3.53	0.063
Interaction	0.01	1	0.12	0.734
Residuals	10.60	108		

4mm Analysis

Figure 2 shows the distributions of thermal spreads of the LigaSure and Voyant devices. The mean LigaSure thermal spread is slightly greater on the right side than on the left (,),

medRxiv preprint doi: https://doi.org/10.1101/2022.09.25.22280350; this version posted December 1, 2022. The copyright holder for this preprint (which was not certified by peer review) is the author/funder, who has granted medRxiv a license to display the preprint in perpetuity. All rights reserved. No reuse allowed without permission.

while the left side is slightly greater than the right side for Voyant (,). The lines connect the sides between the two devices cross, suggesting the possibility of an interaction, although the slopes for each line do not appear to be very distinct.

Figure 2: Mean Thermal Spread by Device and Side

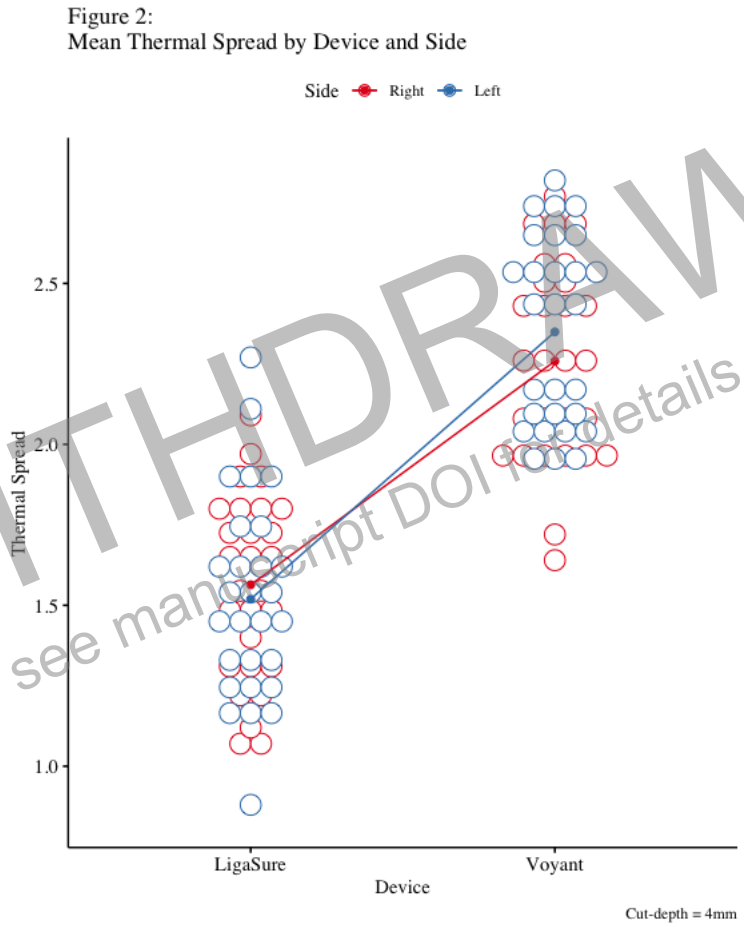

WITHDRAWN
see manuscript DOI for details

Table 2 shows the result of the ANOVA for the cut-depth of 4mm. Despite the evidence in the figures above that there may be an interaction between the factors of side and device, the interaction effect is not significant in the ANOVA results ( ). The main effect of device is once again significant at the level ( ), but the main effect of side is not ( ).

Table 2:
ANOVA Results (Cut-Depth: 4mm)

Term	SS: Type III	DF	F Statistic	P Value
Device	16.28	1	182.37	< 0.001
Side	0.02	1	0.17	0.682
Interaction	0.13	1	1.43	0.235
Residuals	9.64	108		

medRxiv preprint doi: https://doi.org/10.1101/2022.09.25.22280350; this version posted December 1, 2022. The copyright holder for this preprint (which was not certified by peer review) is the author/funder, who has granted medRxiv a license to display the preprint in perpetuity. All rights reserved. No reuse allowed without permission.

Combined Analysis

The third analysis combines the left and right thermal spread measure into a single "total" measure of thermal spread, or the sum of the left and right measures. This analysis treats cut-depth (4mm and 7mm) as an independent variable along with the device type.

Figures 3 shows that the thermal spread for the Voyant device is greater than the thermal spread of the LigaSure device for both cut-depths. While the LigaSure device has a consistent distribution at both cut-depths (,), the Voyant device has a larger mean thermal spread at 7mm ( ) than it does at 4mm ( ).

Figure 3: Mean of Thermal Spread by Device and Cut-Depth

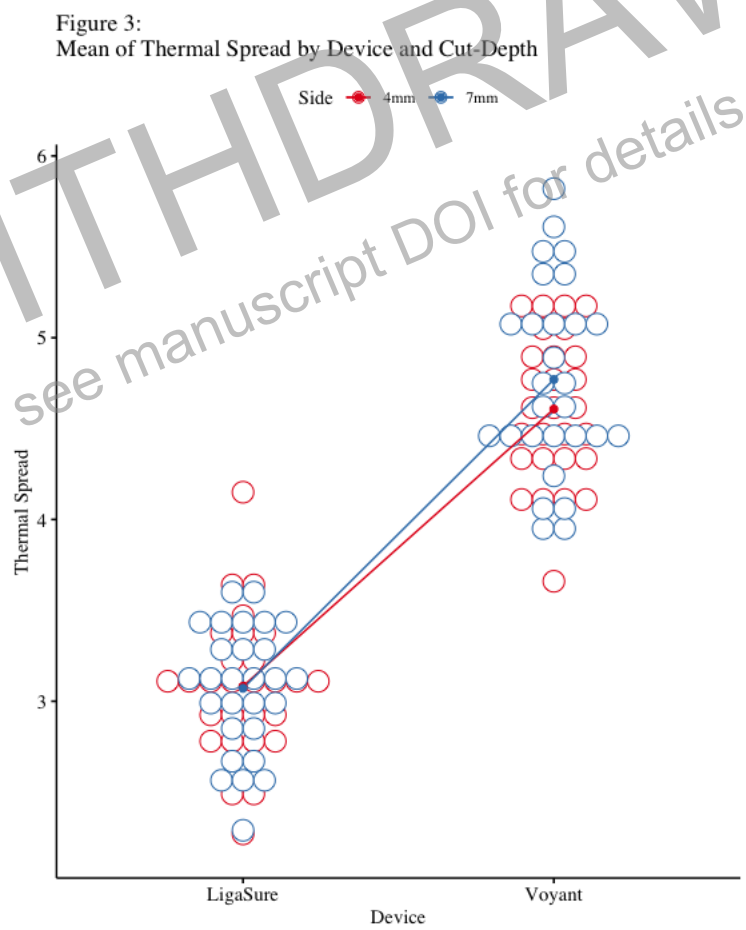

WITHDRAWN
see manuscript DOI for details

Table 3 shows the ANOVA results for the total thermal spread show that there is no interaction between the factors of cut-depth and device ($p = 0.27$). The type of device again has a significant main effect ($p < 0.001$), while the cut-depth does not ($p = 0.34$).

Table 3:
ANOVA Results (Total Thermal Spread)

medRxiv preprint doi: https://doi.org/10.1101/2022.09.25.22280350; this version posted December 1, 2022. The copyright holder for this preprint (which was not certified by peer review) is the author/funder, who has granted medRxiv a license to display the preprint in perpetuity. All rights reserved. No reuse allowed without permission.

Term	SS: Type III	DF	F Statistic	P Value
Device	72.76	1	415.41	< 0.001
Cut-Depth	0.16	1	0.90	0.344
Interaction	0.21	1	1.21	0.274
Residuals	18.92	108		

WITHDRAWN
see manuscript DOI for details

Discussion

LigaSure is an established surgical tool, while Voyant is newer. Previous studies have examined LigaSure versus Harmonic (8), however literature on Voyant is scant. Voyant has become popular because it is more cost effective. Our data suggests that while the side-to-side and cut depth do not impact the thermal spread for either device, LigaSure has significantly less spread overall. This has surgical implications, suggesting that, despite the cost savings posed by Voyant, LigaSure is the preferred instrument.

Previous work demonstrated some differences between the LigaSure 5 mm Blunt Tip and Voyant 5 mm Fusion. Wille et al investigated bursting pressure, sealing time, tissue fusion, thermal spread and radiation, and jaw force for the LigaSure and Voyant 5 mm devices. T-tests were used for analysis and found no difference in bursting pressure, thermal spread, or quality of luminal fusion. Additionally, they report that LigaSure had a faster vessel sealing time, higher jaw force, and lower maximal temperature. (9) Our investigation of thermal spread varies from theirs, and here we report significantly increased thermal spread with the Voyant tool. This difference may be the result of their use of isolated porcine vessels versus our choice of raw pork muscle. Our material was chosen to mimic bowel mesentery. Porcine tissue is commonly used for studying electrocautery. (10) This represents a notable limitation of our study. Future studies could examine human tissues or use appropriate settings by asking the companies to program the devices for the specific tissue being used.

Decreasing thermal spread is important for minimizing damage to surrounding tissues.(3) The current literature on Voyant products is severely lacking compared to literature on LigaSure. We suggest increasing research on the Voyant device in order to more conclusively demonstrate how it compares to LigaSure. These devices are not manufactured for in-vitro use in porcine tissues and we would like to validate our study in a live animal model.

medRxiv preprint doi: https://doi.org/10.1101/2022.09.25.22280350; this version posted December 1, 2022. The copyright holder for this preprint (which was not certified by peer review) is the author/funder, who has granted medRxiv a license to display the preprint in perpetuity. All rights reserved. No reuse allowed without permission.

Data Availability

All data generated or analyzed during this study are included in this published article in the supplementary files.

References

1. Okhunov Z, Yoon R, Lusch A, Spradling K, Suarez M, Kaler KS, et al. evaluation and comparison of contemporary energy-based surgical vessel sealing devices. *J Endourol*. 2018 Apr;32(4):329–37.

2. Olasehinde O, Owojuyigbe A, Adeyemo A, Mosanya A, Aaron O, Wuraola F, et al. Use of energy device in general surgical operations: impact on peri-operative outcomes. *BMC Surg*. 2022 Dec 9;22(1):90.

3. Sankaranarayanan G, Resapu RR, Jones DB, Schwaitzberg S, De S. Common uses and cited complications of energy in surgery. *Surg Endosc*. 2013 Sep 23;27(9):3056–72.

4. FDA. FDA Devices [Internet]. [cited 2022 Sep 21]. Available from: https://www.fda.gov/medical-devices/device-advice-comprehensive-regulatory-assistance/medical-device-databases

5. Hayami M, Watanabe M, Mine S, Imamura Y, Okamura A, Yuda M, et al. Lateral thermal spread induced by energy devices: a porcine model to evaluate the influence on the recurrent laryngeal nerve. *Surg Endosc*. 2019 Dec 7;33(12):4153–63.

6. Smith CT, Zarebczan B, Alhefdhi A, Chen H. Infrared Thermographic profiles of vessel sealing devices on thyroid parenchyma. *J Surg Res.* 2011 Sep;170(1):64–8.

7. Koyanagi K, Kato F, Nakanishi K, Ozawa S. Lateral thermal spread and recurrent laryngeal nerve paralysis after minimally invasive esophagectomy in bipolar vessel sealing and ultrasonic energy devices: a comparative study. *Esophagus*. 2018 Oct 31;15(4):249–55.

8. Sutton PA, Awad S, Perkins AC, Lobo DN. Comparison of lateral thermal spread using monopolar and bipolar diathermy, the Harmonic Scalpel™ and the Ligasure™. Br J Surg. 2010 Feb 5;97(3):428–33.

9. Wille AJ, Speer E, Chow S, Hammill C, Dunst CM, Reavis KM, et al. Comparison of two laparoscopic bipolar electrosurgical devices in a porcine model. SAGES 2015. 2015.

10. Song C, Tang B, Campbell PA, Cuschieri A. Thermal spread and heat absorbance differences between open and laparoscopic surgeries during energized dissections by electrosurgical instruments. *Surg Endosc*. 2009 Nov 19;23(11):2480–7.

WITHDRAWN
see manuscript DOI for details