

Pooled RNA extraction and PCR assay for efficient SARS-CoV-2 detection

Roni Ben-Ami^{1,*}, Agnes Klochendler^{1,*}, Matan Seidel^{2,*}, Tal Sido³, Ori Gurel-Gurevich⁴, Moran Yassour^{5,6}, Eran Meshorer⁷, Gil Benedek⁸, Irit Fogel⁸, Esther Oiknine-Djian⁸, Asaf Gertler⁸, Zeev Rotstein⁸, Bruno Lavi⁸, Yuval Dor^{1,#}, Dana G. Wolf^{8,9,#}, Maayan Salton^{10,#}, Yotam Drier^{9,#}

¹ Department of Developmental Biology and Cancer Research, IMRIC, Faculty of Medicine, The Hebrew University of Jerusalem, Jerusalem, Israel.

² School of Mathematical Sciences, Tel Aviv University, Tel Aviv, Israel.

³ Department of Mathematics, Bar-Ilan University, Ramat-Gan, Israel.

⁴ Einstein Institute of Mathematics, The Hebrew University of Jerusalem, Jerusalem, Israel.

⁵ Department of Microbiology and Molecular Genetics, IMRIC, Faculty of Medicine, The Hebrew University of Jerusalem, Jerusalem, Israel.

⁶ School of Computer Science and Engineering, The Hebrew University of Jerusalem, Jerusalem, Israel.

⁷ Department of Genetics and Edmond and Lily Center for Brain Sciences (ELSC), The Hebrew University of Jerusalem, Jerusalem, Israel.

⁸ Hadassah – Hebrew University Medical Center, Jerusalem, Israel.

⁹ The Lautenberg Center for Immunology and Cancer Research, IMRIC, Faculty of Medicine, The Hebrew University of Jerusalem, Jerusalem, Israel.

¹⁰ Department of Biochemistry and Molecular Biology, IMRIC, Faculty of Medicine, The Hebrew University of Jerusalem, Jerusalem, Israel.

* These authors contributed equally to the work.

These authors contributed equally to the work. Corresponding authors e-mails: yuvald@ekmd.huji.ac.il, danaw@ekmd.huji.ac.il, maayan.salton@mail.huji.ac.il, yotam.drier@mail.huji.ac.il.

Abstract

Testing for active SARS-CoV-2 infection is a fundamental tool in public health measures taken to control the COVID-19 pandemic. Due to the overwhelming use of SARS-CoV-2 RT-PCR tests worldwide, availability of test kits has become a major bottleneck. Here we demonstrate the reliability and efficiency of two simple pooling strategies that can increase testing capacity about 5-fold to 7.5-fold, in populations with a low infection rate. We have implemented the method in a routine clinical diagnosis setting, and already tested 2,168 individuals for SARS-CoV-2 using 311 RNA extraction and RT-PCR kits.

Introduction

An emerging novel severe acute respiratory syndrome-related coronavirus, SARS-CoV-2, is the virus behind the global COVID-19 pandemic. Among the foremost priorities to facilitate efficient public health interventions is a reliable and accessible diagnosis of an active SARS-CoV-2 infection. The standard laboratory diagnosis of COVID-19 involves three main steps, namely, viral inactivation and lysis of the nasopharyngeal swab sample, extraction (or purification) of viral RNA, and reverse transcription (RT)-PCR. Due to the rapid spread of the virus and the increasing demand for tests, the limited availability of test reagents, mainly RNA extraction kits, has become (and is likely to continue to be) a major bottleneck as the pandemic expands.

Of particular importance is the ability to survey large asymptomatic populations- (1) to trace asymptomatic COVID-19 carriers which are otherwise difficult to identify and isolate; (2) to assure key personnel (e.g. healthcare personnel) are not contagious; (3) to accurately estimate the spread of the infection and the effectiveness of community measures and social distancing; and (4) to allow and monitor a safe return to work. Clearly, more efficient and higher-throughput diagnostic approaches are needed to support such efforts.

Several attempts to address this challenge have already been suggested, that can be categorized into three major approaches. The first approach is to replace PCR based methods by other direct diagnostic methods such as Loop-mediated Isothermal Amplification (LAMP) [1–3] and CRISPR based diagnostic tools [4–6], the second approach involves serological surveys [7–10], and the third approach involves the improvement of the PCR methods capacity by optimization and automation (e.g. [11–13]) or by reducing the required number of tests via pooling samples together, known as group testing.

Group testing is a field of research in the intersection of mathematics, computer science and information theory, with applications in biology, communication and more. A group testing algorithm is a testing scheme which is directed towards minimizing the number of tests conducted on a set of samples by using the ability to test pooled subsets of samples. If a pool of n samples tests negative, all samples must be negative, and therefore their status has been determined in only one test instead of n individual tests. Various group testing algorithms exist, with different assumptions and constraints (see [14,15]). While many such algorithms, most notably binary splitting, may be very efficient in theory, they might be unsuitable because of practical limitations. Three such limitations might be: (1) a limit on the number of stages due to the importance of delivering a test result quickly, exemplified by the urgent clinical context of COVID-19 diagnosis; (2) a limit on the ability to dilute samples and still safely identify a single positive sample in a pool; (3) favorability of simple algorithms which may minimize human error in a laboratory setting.

While several pooling approaches for SARS-CoV-2 detection were recently suggested (e.g. [16–19]), none demonstrated adherence to current clinical standards, nor shown to work for performing RNA extraction in pools, which is typically the limiting step. Here we describe and demonstrate practical pooling solutions that save time and reagents by performing RNA extraction and RT-PCR on pooled samples. Unlike other suggestions of large-

scale pooling and non-PCR-based methods, we maintain comparable sensitivity, and therefore the method complies with current clinical requirements. The simplicity of the method, similarity to currently approved procedures, and the fact that we do not require special sample handling or additional information make it easily adoptable on a large scale. We offer two such pooling approaches, based either on simple (Dorfman) pooling or matrix pooling [20,21], and demonstrate their efficiency and sensitivity in the daily reality of SARS-CoV-2-infected clinical cases. Under current clinical diagnosis parameters these methods allow 5-fold to 7.5-fold increase in throughput when applied to populations with < 1% positives, including screened asymptomatic healthcare personnel and essential industries' employees.

Results

At the Hadassah Medical Center, two distinct populations of people are tested for SARS-CoV-2 at present. First, we receive samples from symptomatic patients, from the hospital and from the community. In these samples, about 10% of SARS-CoV-2 tests are positive. Second, we receive samples from prospectively screened asymptomatic populations such as hospital employees and workers in essential industries. Among the latter, individual testing of >2,000 samples revealed that the rate of positives ranged between 0.1% and 1%. Based on these findings, we examined the feasibility of pooled testing for asymptomatic populations, and designed appropriate pooling strategies.

A key requirement of pooled RNA extraction and RT-PCR tests is to retain sufficient sensitivity. In our RT-PCR assay, a sample is defined as *positive* if the viral genome is detected at threshold cycle (Ct) values ≤ 35 , as *indeterminate* at Ct values >35 and ≤ 38 , and as *negative* at Ct values >38 . Theoretically, pooling 8 samples should elevate the Ct of a single positive sample by 3 cycles, and pooling 16 samples should elevate the Ct by 4 cycles. However, reproducibility of RNA extraction and RT-PCR might be affected by other factors. We therefore empirically tested the assay sensitivity, when multiple negative samples and one positive sample were mixed at the lysate stage. As shown in **Figure 1**, positive samples were readily detected, even when their individual Ct ranged between 35 and 38. Thus, SARS-CoV-2 RNA can be reliably detected in pooled samples without compromising the assay sensitivity.

The first pooling strategy is a simple two-stage testing algorithm known as Dorfman pooling [22]. In the first stage, the samples are divided into disjoint pools of n samples each, and each such pool is tested. A negative result implies that all samples in the pool are negative, while a positive result implies that at least one sample in the pool is positive. In the second stage, the samples of each pool that tested positive are individually tested. While such approaches for SARS-CoV-2 have been recently suggested (e.g. [16,17]), we have tested direct pooling of lysates of clinical nasopharyngeal samples, with RNA extraction already performed on the pooled samples. First, we tested the pooling of 184 consecutive samples into 23 pools of 8 samples each, and also tested in parallel each sample individually. This approach yielded highly accurate results, with no loss of diagnostic assay sensitivity:

each of the pools that contained one or more positive samples was found to be positive, and all the pools that contained only negative samples were found to be negative (**Figure 1**). Of the 5 pools which contained one individual sample with an “indeterminate” result (in each pool), one was found to be negative suggesting potential yet negligible loss of sensitivity.

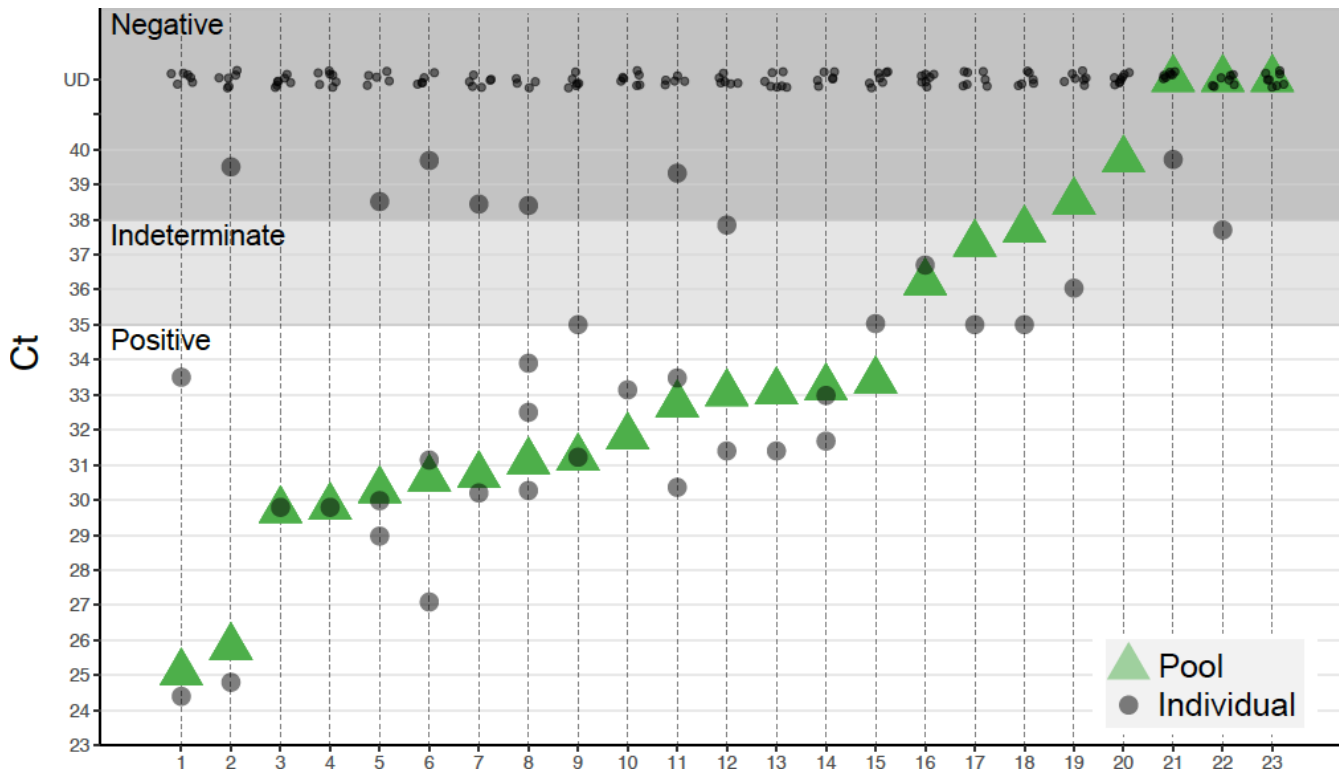


Figure 1: Pooling 8 lysates retain clinical sensitivity. Shown are results of 23 pooling experiments, with 8 lysates in each pool; 15 pools with positive samples indeed come up positive (pools 1-15), 3 pools without positive samples come up negative (pools 20, 21, 23), and 4 out of 5 pools containing a single indeterminate sample detected as indeterminate (pools 16, 17, 18, 19, 22); Pools containing 1-2 samples with low amount of SARS-CoV-2 are detected at a similar Ct (pools 9-18), showing clinical sensitivity is retained and the risk of false negatives is minimal. UD= Undetected.

To further reduce the need to retest positive pools we have also tested a two-stage matrix pooling strategy [20,21], where n^2 samples are ordered in an $n \times n$ matrix. Each row and each column are pooled, resulting in $2n$ tests, $\frac{1}{2}n$ times less tests than individual testing. If either the number of positive rows or columns is one, the positive samples can be uniquely identified at the intersections of the positive rows and columns. Otherwise, if both the number of positive rows and columns is greater than one, intersections of positive rows and columns will be retested individually. We have tested this approach with pooling 75 samples into three 5×5 matrices, and identified all positive samples accurately (**Figure 2**). Importantly, the positive samples were detected in both the row and the column pools at a similar cycle in all three tested matrices, suggesting the pooling scheme is robust.

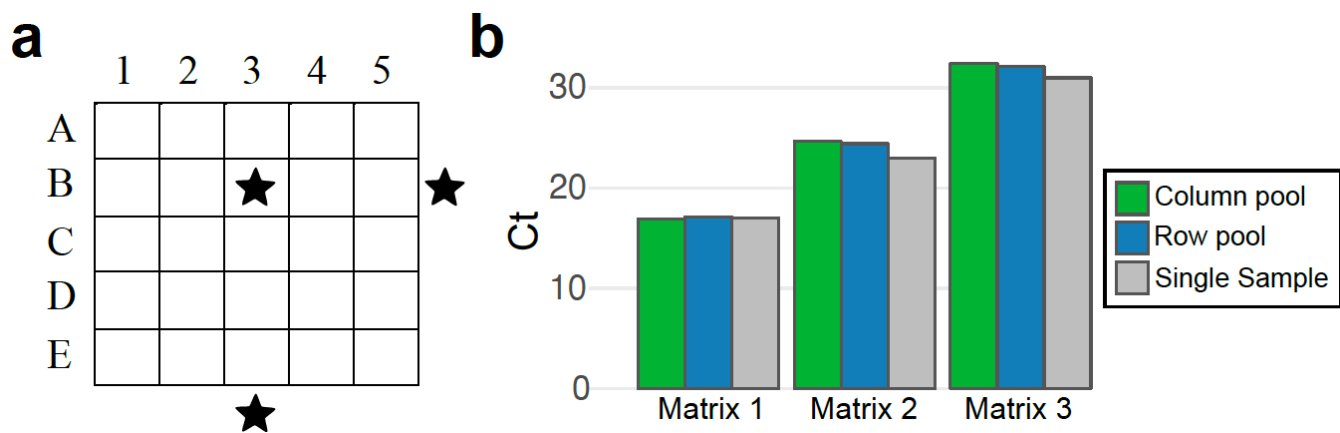


Figure 2: matrix pooling. (a) Scheme for 5x5 matrix pooling. 25 samples sorted in a 5 x 5 matrix and each row and each column is pooled into a total of 10 pools, on which RNA extraction, reverse transcription and qPCR are performed. In this illustration row B and column 3 are positive (black stars), hence sample B3 is the only positive sample. If more than one row and one column are positive then all the samples in the intersection need to be retested, as some may be negative. (b) Three 5x5 pool matrices were generated (30 pools from 75 lysates). Each matrix (25 lysates that were previously tested individually) included a single lysate positive for SARS-COV-2. As expected, only 6 pools (one row and one column per matrix) were positive for SARS-COV-2, while 24 pools had Ct >40 (Undetected). RT-PCR Ct values of positive pools were nearly identical in the column pool (green) and the row pool (blue), and similar to the values of the individual test of the positive sample (gray).

	No. of samples	No. of pools	No. of positive pools	Ct of positive pools	No. of <u>positive</u> individual samples in the positive pools	Ct of positive individual samples	No. of total tests	No. of tests saved, compared to single sample tests (%)
Pool batch 1	720	90	1	21.8	1	19.4	98	622 (86.4)
Pool batch 2	720	90	0	-	-	-	90	630 (87.5)
Pool batch 3	728	91	3 positives, 1 indeterminate	25.39	2	22.05, 28.72	123	605 (83.1)
				37.44	1	37.67*		
				35.26	1	34.66		
				38.67 indeterminate	0	38.24 (determined as negative)		

Table 1: Summary of pooled tests run at the Hadassah Medical Center. Ct- cycle threshold.

* According to the hospital's protocol for indeterminate values, RT-PCR was repeated with a different kit, and eventually was determined as positive.

Given the successful validation of both pooling strategies, we have adopted a Dorfman pooling protocol of 1:8 and employed it for the routine testing of nasopharyngeal swab samples from screened asymptomatic healthcare

personnel and employees of essential industries. Individual barcoded samples were received at the laboratory, inactivated by lysis buffer, pooled on a Tecan liquid-handling robot, and the pools were processed on a Qiasymphony robot for RNA extraction, and analyzed by RT-PCR. Results were interpreted and samples in positive pools were subsequently individually tested. Note that analysis of pool results requires close attention to indeterminate-result pools, showing a signal at $35 < Ct < 38$, as these may contain individual positive samples. Therefore, criteria for retesting pools must be more stringent, e.g. a signal with $Ct \sim 38$ would be defined as negative when individual samples are tested, but warrants re-testing of individual samples when encountered in a pool (see **Table 1**, batch 3).

At the time of submission of this manuscript, we have already tested 2,168 samples by pooling, thereby using 311 RNA extraction and RT-PCR reactions (a mere 14% of kits that would have been used in the full individual testing). Among these samples, we have identified and individually validated five positive samples, corresponding to a rate of 0.23% (**Table 1**).

Discussion

Here we have demonstrated reliable and efficient diagnosis of SARS-CoV-2 infections in pooled samples, when pooling is done immediately after lysis, and RNA extraction, reverse transcription and PCR are performed on the pooled lysates. This saves time, work and reagents, allowing a considerable throughput increase of clinical diagnostic labs and opening the door for screens in largely healthy populations. Specifically, we have demonstrated that pooling lysates from 5 or 8 nasopharyngeal swab samples retains the sensitivity of viral RNA detection, allowing identification of SARS-CoV-2-positive individuals.

An important consideration before implementing group testing is the expected rate of false positive and false negative results. Based on our experience with >2000 samples from asymptomatic individuals, we did not encounter any false positives in the pools, as shown in **Figure 1** and **Table 1**. False negatives are in principle more worrisome when testing in pools, because samples that failed at the RNA extraction step will be missed (while our individual testing includes amplification of a human transcript serving as an internal control for proper RNA extraction and RT-PCR of each sample). To define the magnitude of this potential problem, we examined a set of 13,781 tests done at our center, which were all expected to show a signal for a human gene serving as internal assay control. Amplification of the human gene failed in 52 samples (0.38% of the cases). Thus, we estimate that our current protocol of pooled sampling carries a risk of missing 0.38% of the positive samples. In a population of 1,000,000 individuals tested, of which 1,000 are positive (rate of 0.1%), this predicts that 4 positive individuals will be missed when using pools. We posit that this is a tolerable situation, particularly given the potentially much higher rates of false negative results due to swab sampling and other errors upstream.

We define the *efficiency* of a pooling algorithm as the total number of samples divided by the expected number of tests conducted on them. We assume all samples are independent and identically distributed, and denote the

probability of a sample to be positive by p (prevalence of detectable COVID-19 patients in the relevant population) and the pool size by n . The efficiency of the algorithms described above depends on both p and n . The best theoretical efficiency is $(-p \log_2(p) - (1-p) \log_2(1-p))^{-1}$ [23]. The efficiency of Dorfman pooling is $(1 + 1/n - (1-p)^n)^{-1}$ [22]. We chose a pool size of $n=8$ samples as it allows low false negative rate (**Figure 1**) and high efficiency for a wide range of COVID-19 prevalence (**Table 2**). The prevalence of detectable COVID-19 in an asymptomatic population is estimated to be considerably below 1%, and indeed of the 2168 asymptomatic subjects tested in the present study only 0.23% were found positive. Therefore, efficiency is likely to be 5 - 7.5. For higher prevalence the efficiency of matrix pooling is somewhat higher (see **Table 2** and supplementary note). We provide a tool (https://github.com/matanseidel/pooling_optimization) to help choose the approach and pool size based on the prevalence. Even when matrix pooling is not more efficient, it may have other benefits, as it significantly reduces the need for retesting, and provides additional confidence that a sample is negative as it is detected as negative in two pools.

Prevalence (p)	0.1%	1%	2%	5%	10%	20%
Maximal theoretical efficiency	87.7	12.4	7.1	3.5	2.13	1.39
Dorfman $n=8$ efficiency	7.5	4.9	3.6	2.2	1.44	1.04
Matrix $n=8$ efficiency	4.0	3.9	3.6	2.6	1.68	1.05

Table 2: Efficiency of Dorfman and matrix pooling with pool size $n=8$ compared with optimal efficiency.

In the case that samples are not independent, and we have information regarding their dependency, we can try to further efficiency by grouping together dependent samples, that is, samples that are likely all positives or all negatives, such as members of the same family, or samples that are likely to be all negative since they have a low risk profile. This will increase the number of negative pools, and therefore decrease the overall number of tests conducted.

The prevalence of COVID-19 in the tested population is not always known, which could affect the optimal pool size. This could be addressed either by other external estimates, such as a previous run of individual samples, rate of symptomatic patients, or alternative methods such as serological screening or wastewater titers monitoring [24]. Alternatively, it is possible to dynamically adapt pooling sizes, when the measured rate of positive samples is different than expected. Finally, there exist some group testing algorithms [15,25] for the purpose of estimating the number of positive samples while using a relatively small (logarithmic) amount of tests, and such algorithms may be adapted to clinical constraints and parameters.

Future improvement of the sensitivity of the test, such as better sets of primers, improved sample collection and inclusion of information about pre-test probability will allow retaining sensitivity even when pooling a large number of sample lysates together. This will enable further improving efficiency, especially when prevalence is low, by increasing the pool size.

In summary, we demonstrate in a real-life situation the usefulness of pooled sampling starting at the early lysate stage. This allows for reliable and efficient screening of large asymptomatic populations for the presence of SARS-CoV-2 infection, even when RNA extraction and RT-PCR reagents are in short supply.

Methods

Sample collection, RNA extraction and RT-PCR Detection

Nasopharyngeal swab samples were collected in 2 ml Viral Transport Medium (VTM) and mixed 1:1 with a 2x concentrated Zymo lysis buffer, or collected directly to 2 ml Zymo lysis buffer. For the initial validation, samples were collected from symptomatic patients or from screened healthy asymptomatic subjects. For sample lysate preparation 220 μ L of sample VTM were added to 280 μ L lysis buffer. RNA was extracted using MagNA Pure 96 kit (Roche Lifesciences) using Roche platform and eluted in 60 μ L. Ten μ L of RNA was used in 30 μ L reaction using Real-Time Fluorescent RT-PCR kit (BGI).

Pool RNA extraction and RT-PCR Detection

For matrix pool design we pooled equal volumes of sample lysate from each of the subjects to a final volume of 450 μ L and used MagNA Pure 96 kit (Roche Lifesciences) using Roche platform. As supply was limited for this kit, we have used QIASymphony DSP Virus/Pathogen kit on Qiasymphony platform for 1:8 pool design. We pooled equal volumes of sample lysate from each of the subjects to a final volume of 400 μ L. Positive 1:8 pools were validated by single tests using QIASymphony RNA kit on Qiasymphony platform. Both Qiagen kits were used with Zymo lysis buffer, and therefore we skipped the lysis and Proteinase K step. RNA was eluted into 60 μ L; 10 μ L of RNA was used for a 30 μ L reaction using Real-Time Fluorescent RT-PCR kit (BGI).

References

1. Zhang Y, Odiwuor N, Xiong J, Sun L, Nyaruaba RO, Wei H, et al. Rapid Molecular Detection of SARS-CoV-2 (COVID-19) Virus RNA Using Colorimetric LAMP. *Infectious Diseases (except HIV/AIDS)*. medRxiv; 2020. doi:10.1101/2020.02.26.20028373
2. Yan C, Cui J, Huang L, Du B, Chen L, Xue G, et al. Rapid and visual detection of 2019 novel coronavirus (SARS-CoV-2) by a reverse transcription loop-mediated isothermal amplification assay. *Clin Microbiol*

Infect. 2020. doi:10.1016/j.cmi.2020.04.001

3. Park G-S, Ku K, Baek S-H, Kim S-J, Kim SI, Kim B-T, et al. Development of Reverse Transcription Loop-mediated Isothermal Amplification (RT-LAMP) Assays Targeting SARS-CoV-2. *J Mol Diagn*. 2020. doi:10.1016/j.jmoldx.2020.03.006
4. Ai J-W, Zhang Y, Zhang H-C, Xu T, Zhang W-H. Era of molecular diagnosis for pathogen identification of unexplained pneumonia, lessons to be learned. *Emerg Microbes Infect*. 2020;9: 597–600.
5. Lucia C, Federico P-B, Alejandra GC. An ultrasensitive, rapid, and portable coronavirus SARS-CoV-2 sequence detection method based on CRISPR-Cas12. *bioRxiv*. 2020. p. 2020.02.29.971127. doi:10.1101/2020.02.29.971127
6. Broughton JP, Deng X, Yu G, Fasching CL, Singh J, Streithorst J, et al. Rapid Detection of 2019 Novel Coronavirus SARS-CoV-2 Using a CRISPR-based DETECTR Lateral Flow Assay. *Infectious Diseases (except HIV/AIDS)*. medRxiv; 2020. doi:10.1101/2020.03.06.20032334
7. Guo L, Ren L, Yang S, Xiao M, Chang D, Yang F, et al. Profiling Early Humoral Response to Diagnose Novel Coronavirus Disease (COVID-19). *Clin Infect Dis*. 2020. doi:10.1093/cid/ciaa310
8. Xiao S-Y, Wu Y, Liu H. Evolving status of the 2019 novel coronavirus infection: Proposal of conventional serologic assays for disease diagnosis and infection monitoring. *Journal of medical virology*. 2020. pp. 464–467.
9. Zhang W, Du R-H, Li B, Zheng X-S, Yang X-L, Hu B, et al. Molecular and serological investigation of 2019-nCoV infected patients: implication of multiple shedding routes. *Emerg Microbes Infect*. 2020;9: 386–389.
10. Lassaunière R, Frische A, Harboe ZB, Nielsen ACY, Fomsgaard A, Krogfelt KA, et al. Evaluation of nine commercial SARS-CoV-2 immunoassays. *Infectious Diseases (except HIV/AIDS)*. medRxiv; 2020. doi:10.1101/2020.04.09.20056325
11. Fomsgaard AS, Rosenstjerne MW. An alternative workflow for molecular detection of SARS-CoV-2 - escape from the NA extraction kit-shortage. medRxiv. 2020; 2020.03.27.20044495.
12. Barra GB, Santa Rita TH, Mesquita PG, Jacomo RH, Nery LFA. Analytical sensibility and specificity of two RT-qPCR protocols for SARS-CoV-2 detection performed in an automated workflow. *Infectious Diseases (except HIV/AIDS)*. medRxiv; 2020. doi:10.1101/2020.03.07.20032326
13. Kalikiri MKR, Hasan MR, Mirza F, Xaba T, Tang P, Lorenz S. High-throughput extraction of SARS-CoV-2 RNA from nasopharyngeal swabs using solid-phase reverse immobilization beads. *Infectious Diseases (except HIV/AIDS)*. medRxiv; 2020. doi:10.1101/2020.04.08.20055731
14. Du D, Hwang FK, Hwang F. *Combinatorial Group Testing and Its Applications*. World Scientific; 2000.

15. Aldridge M, Johnson O, Scarlett J. Group Testing: An Information Theory Perspective. *Foundations and Trends® in Communications and Information Theory*. 2019;15: 196–392.
16. Yelin I, Aharony N, Shaer-Tamar E, Argoetti A, Messer E, Berenbaum D, et al. Evaluation of COVID-19 RT-qPCR test in multi-sample pools. *Infectious Diseases (except HIV/AIDS)*. medRxiv; 2020. doi:10.1101/2020.03.26.20039438
17. Sinnott-Armstrong N, Klein D, Hickey B. Evaluation of Group Testing for SARS-CoV-2 RNA. *Infectious Diseases (except HIV/AIDS)*. medRxiv; 2020. doi:10.1101/2020.03.27.20043968
18. Shani-Narkiss H, Gilday OD, Yayon N, Landau ID. Efficient and Practical Sample Pooling High-Throughput PCR Diagnosis of COVID-19. *Public and Global Health*. medRxiv; 2020. doi:10.1101/2020.04.06.20052159
19. Deckert A, Bärnighausen T, Kyei N. Pooled-sample analysis strategies for COVID-19 mass testing: a simulation study. nCoV. World Health Organization; 2020.
20. Kwiatkowski TJ Jr, Zoghbi HY, Ledbetter SA, Ellison KA, Chinault AC. Rapid identification of yeast artificial chromosome clones by matrix pooling and crude lysate PCR. *Nucleic Acids Res*. 1990;18: 7191–7192.
21. Barillot E, Lacroix B, Cohen D. Theoretical analysis of library screening using a N-dimensional pooling strategy. *Nucleic Acids Res*. 1991;19: 6241–6247.
22. Dorfman R. The Detection of Defective Members of Large Populations. *Ann Math Stat*. 1943;14: 436–440.
23. Li T, Chan CL, Huang W, Kaced T, Jaggi S. Group testing with prior statistics. 2014 IEEE International Symposium on Information Theory. 2014. pp. 2346–2350.
24. Wu F, Xiao A, Zhang J, Gu X, Lee WL, Kauffman K, et al. SARS-CoV-2 titers in wastewater are higher than expected from clinically confirmed cases. medRxiv. 2020; 2020.04.05.20051540.
25. Damaschke P, Sheikh Muhammad A. Competitive Group Testing and Learning Hidden Vertex Covers with Minimum Adaptivity. *Fundamentals of Computation Theory*. Springer Berlin Heidelberg; 2009. pp. 84–95.