

## **Supporting Information**

### **A Digital CRISPR-based Method for the Rapid Detection and Absolute Quantification of Viral Nucleic Acids**

Xiaolin Wu<sup>1</sup>, Cheryl Chan<sup>1</sup>, Yie Hou Lee<sup>1</sup>, Stacy L. Springs<sup>1,2</sup>, Timothy K. Lu<sup>1,3,4,5,6,7,8\*</sup>, Hanry Yu<sup>1,9,10,11\*</sup>

<sup>1</sup>Singapore-MIT Alliance for Research and Technology, Critical Analytics for Manufacturing of Personalized Medicine Interdisciplinary Research Group, Singapore 138602, Singapore

<sup>2</sup> Center for Biomedical Innovation, Massachusetts Institute of Technology, Cambridge, MA, USA.

<sup>3</sup>Synthetic Biology Center, Massachusetts Institute of Technology (MIT), Cambridge, MA 02139, USA

<sup>4</sup>Synthetic Biology Group, Research Laboratory of Electronics, Massachusetts Institute of Technology (MIT), Cambridge, MA 02139, USA

<sup>5</sup>Broad Institute of MIT and Harvard, Cambridge, MA 02142, USA

<sup>6</sup>Department of Electrical Engineering and Computer Science, Massachusetts Institute of Technology (MIT), Cambridge, MA 02142, USA

<sup>7</sup>Harvard-MIT Division of Health Sciences and Technology, Cambridge, MA 02139, USA

<sup>8</sup>Department of Biological Engineering, Massachusetts Institute of Technology (MIT), Cambridge, MA 02142, USA

<sup>9</sup>Institute of Bioengineering and Nanotechnology, A\*STAR, The Nanos, #04-01, 31 Biopolis Way, Singapore 138669, Singapore

<sup>10</sup>Mechanobiology Institute, National University of Singapore, T-Lab, 5A Engineering Drive 1, Singapore 117411, Singapore

<sup>11</sup>Department of Physiology, National University of Singapore, MD9 #03-03, 2 Medical Drive, Singapore 117597, Singapore

\* Correspondence should be addressed to Timothy K. Lu (timlu@mit.edu) and Hanry Yu (phsyuh@nus.edu.sg).

**Table S1. Primers and probes used in this study.**

Name	Sequence	Application
ssDNA-FQ reporter	/56-FAM/TTATT/3IABkFQ/	Cas12a FQ reporter
N-RNA-F	gaaatTAATACGACTCACTATAggg ATGTCTGATAATGGACCCAAAA T	Amplify N gene on plasmid
N-RNA-R	gaaatTTAGGCCTGAGTTGAGTCA GCACT	Amplify N gene on plasmid
CHNCDC-geneN-F	GGGGAACTTCTCCTGCTAGAAT	dPCR Primer for N gene
CHNCDC-geneN-R	CAGACATTTGCTCTCAAGCTG	dPCR Primer for N gene
CHNCDC-geneN-P	/56-FAM/TT GCT GCT G/ZEN/C TTG ACA GAT T/3IABkFQ/	dPCR Probe for N gene
T7-3G IVT primer	GAAATTAATACGACTCACTATAG GG	universal primer used for crRNA synthesis
N-N-RPA-F	AACTCCAGGCAGCAGTAGGGGA ACTT	CRISPR Primer for N gene
N-N-RPA-R	CCTTACCAGACATTTGCTCTC AAG	CRISPR Primer for N gene
N-N-crRNA-IVT	AATCTGTCAAGCAGCAGATCTAC ACTTAGTAGAAATTACCCCTATAG TGAGTCGTATTAATTTC	crRNA template for N gene, pair with T7-3G IVT primer
N-AIOD-F <sup>1</sup>	AGGCAGCAGTAGGGGAACCTCT CCTGCTAGAAT	digital CRISPR Primer for N gene
N-AIOD-R <sup>1</sup>	TTGGCCTTACCAGACATTTGC TCTCAAGCTG	digital CRISPR Primer for N gene
N-AIOD-crRNA-IVT-F	ggctggcaatggcggtgatgATCTACACT TAGTAGAAATTACCCCTATAGTGA GTCGTATTAATTTC	crRNA template for N gene, pair with T7-3G IVT primer

T7-Cas12scaffold-F	gaaatTAATACGACTCACTATAAGG TAATTCTACTAAGTGTAGAT	universal primer used for crRNA synthesis
N-RPA-RR	AGCAGATTCTTAGTGACAGTTT GGCCTTGTG	CRISPR Primer for N gene
N2-RPA-RR	AGCAAAATGACTTGATCTTGAA ATTGGATCT	CRISPR Primer for N gene
N-JQ217-F <sup>2</sup>	CAACTTCCTCAAGGAACAAACATT GCCAAAA	CRISPR Primer for N gene
N-JQ235-R <sup>2</sup>	TGGAGTTGAATTCTTGAAGTGT TGCGACT	CRISPR Primer for N gene
NF-CoV-RR	GAGAAGTTCCCCTACTGCTG	CRISPR Primer for N gene
NF-crRNA-1F	CTTCTACGCAGAAGGGAGCAatct acacttagtagaaatta	crRNA template for N gene, pair with T7-Cas12scaffold-F
EBV-EBNA1-F2	GCCGGTGTGTCGTATATGGAG GTAGTAAGAC	digital CRISPR Primer for EBV
EBV-EBNA1-R2	ATTCCAAGGGAGACGACTCA ATGGTGAA	digital CRISPR Primer for EBV
EBNA-2R1-crRNAR	ACGACATTGTGGAYAGCAAGG atctacacttagtagaaatta	crRNA template for EBV, pair with T7-Cas12scaffold-F


**Table S2. Quantification of linearized plasmid target by dCRISPR**

Number of replications	dPCR measured concentration (copies/µL)	Mean of dCRISPR measured concentration (copies/µL)	Standard deviation (copies/µL)	Relative standard deviation or coefficient of variation (CV)
10	Non template control	0.17	0.15	-
14	0.70	0.60	0.29	49.41%


14	2.80	2.20	0.25	11.25%
13	11.19	9.06	1.23	13.53%
14	44.76	35.53	5.30	14.91%
10	179.06	146.90	18.02	12.27%
10	716.24	626.58	73.96	11.80%
10	2387.46	2027.27	152.76	7.54%

**Table S3. Comparison of digital CRISPR assay with other viral detection methods.**


	RT-PCR	CRISPR-based isothermal method	RT-digital PCR	Digital RPA/digital LAMP	Digital CRISPR
<b>Detecting Substance</b>	RNA, DNA, cDNA	RNA, DNA, cDNA	RNA, DNA, cDNA	DNA, cDNA	DNA, cDNA
<b>LoD (for SARS-CoV-2)</b>	5 copies per reaction	20 copies per reaction	2 copies per reaction	NA	13.5 copies per reaction (0.897 copies/µL in 15 µL reaction)
<b>Result Time</b>	2 hours	<b>1 hour</b>	4 hours	<b>1 hour</b>	<b>1 hour</b>
<b>Thermal cycling Requirements</b>	Yes	<b>No</b>	Yes	<b>No</b>	<b>No</b>
<b>All devices and regents commercially available</b>	Yes	Yes	Yes	No	<b>Yes</b>
<b>Ease of primer and crRNA design</b>	Yes	Moderate	Yes	Moderate	<b>Yes</b>
<b>Specificity</b>	Good	Good	Good	Normal	Good
<b>Absolute quantification</b>	No	No	Yes	Yes	<b>Yes</b>

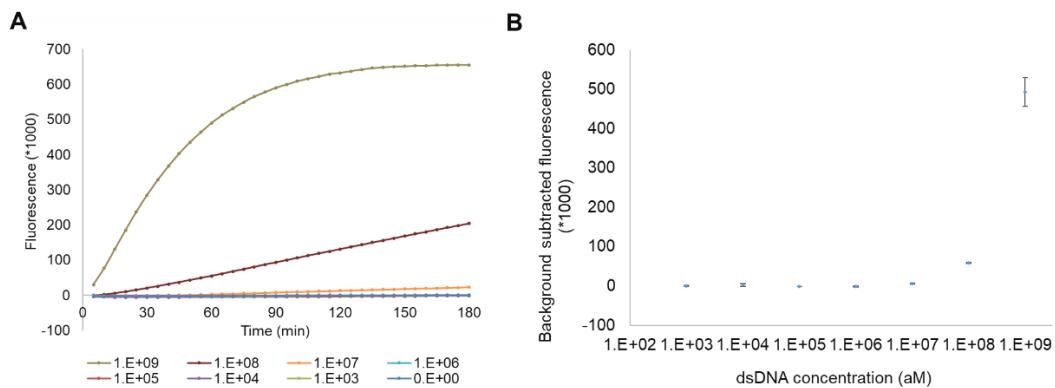


**Figure S1. Cas12a detection sensitivity of dsDNA dilution series without pre-amplification.** **A.** Kinetics of Cas12a-crRNA on dsDNA dilution series. **B.** Detection sensitivity analysis of dsDNA dilution series with Cas12a-crRNA in 1h. 50nM Cas12-crRNA and 250 nM FQ-ssDNA probe were incubated with dsDNA dilution series at 37°C and fluorescence was monitored every 5 min.

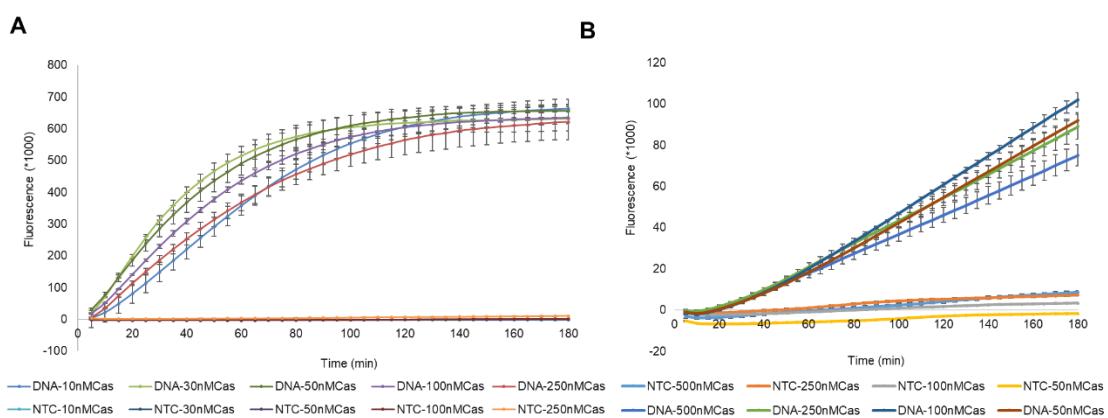


**Figure S2. Detection of dsDNA without preamplification at different Cas12a/crRNA concentrations.** **A.** 1 nM dsDNA incubated with 10-250 nM Cas12a-crRNA and 250 nM FQ ssDNA probe. **B.** 0.1 nM dsDNA incubated with 50-500 nM Cas12a-crRNA and 500 nM FQ ssDNA probe.

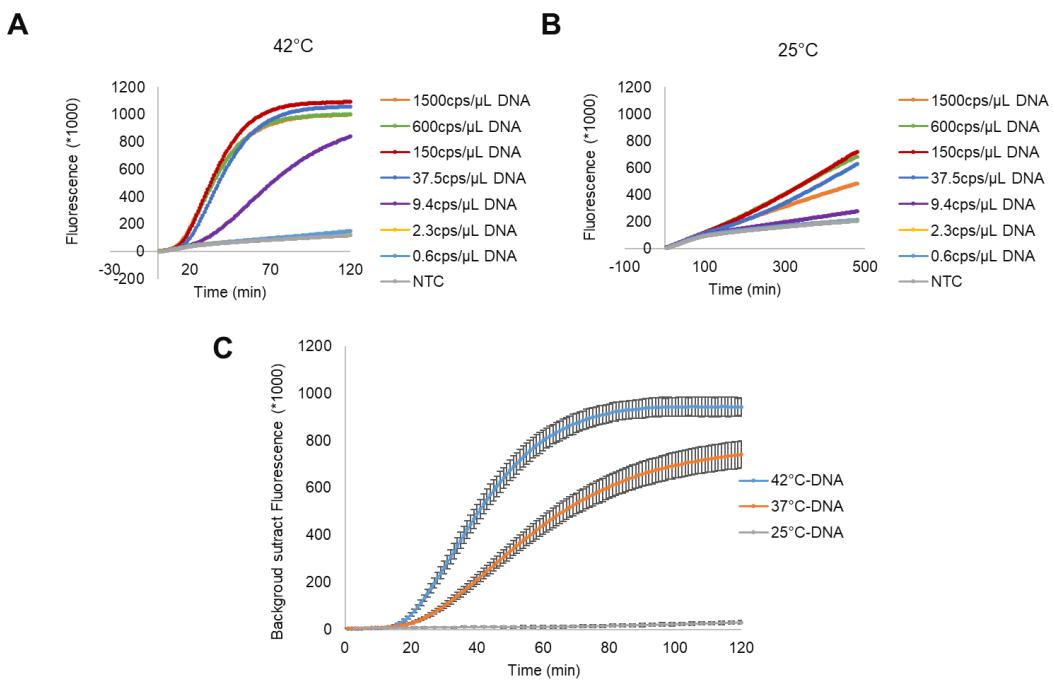


**Figure S3. RPA+Cas12a bulk reaction at different temperatures. A and B.** RPA+Cas12a one-pot reaction on serial dilutions of DNA at 42°C (A) or 25°C (B). **C.** RPA+Cas12a one-pot reaction on 37.5 copies/μL plasmid DNA at different temperatures (25°C, 37°C, and 42°C).

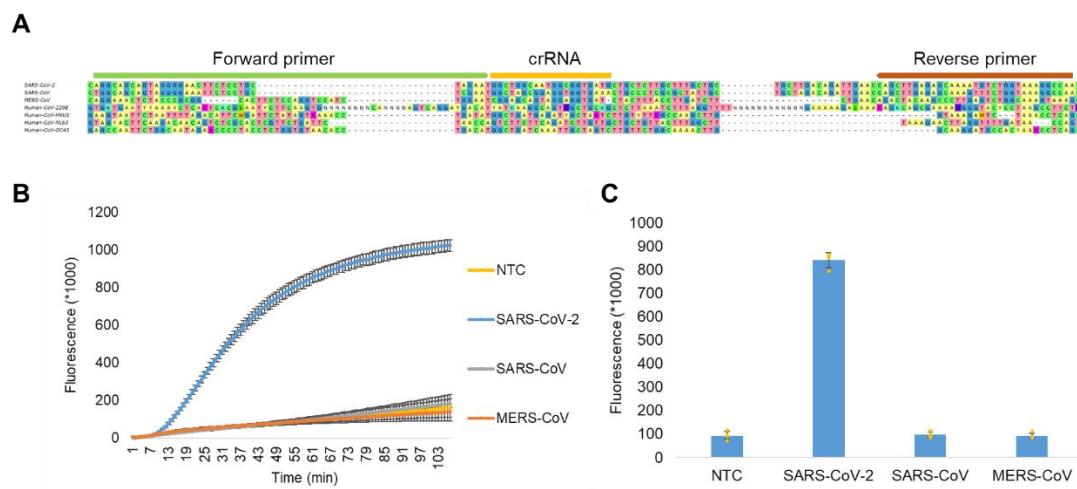

**Figure S4. Specificity analysis for SARS-CoV-2. A.** Sequence alignment of the SARS-CoV-2 target region (N gene) and the corresponding regions on other human coronaviruses. **B.** Time course reaction of bulk RPA-Cas12a assay on SARS-CoV-2, SARS-CoV, and MERS-CoV N gene DNA target. The same concentration (25000 copies/μL) of the N gene target from different coronaviruses was tested by the bulk RPA-Cas12a assay. **C.** Specificity of the bulk RPA-Cas12a assay for detection of the SARS-CoV-2 N gene.

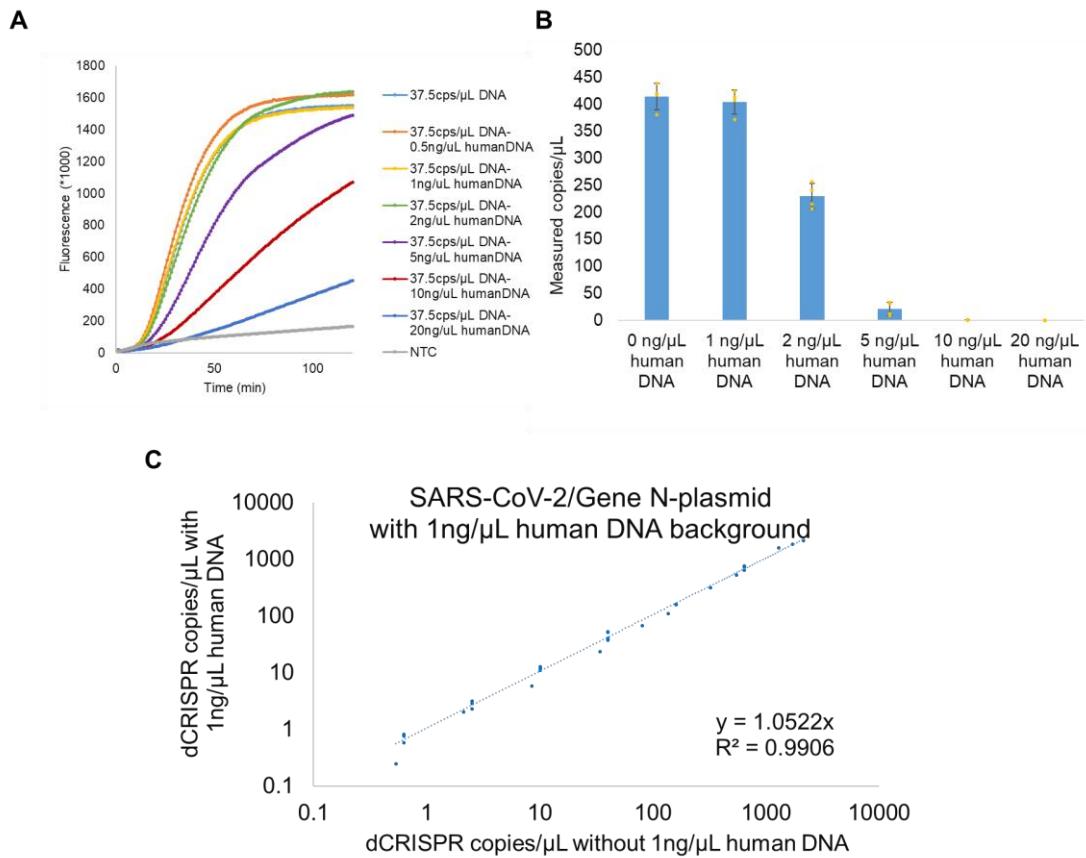

**Figure S5. RPA inhibition by human background DNA. A.** Results of bulk RPA-Cas12a reaction to detect target DNA (i.e., the N gene from SARS-CoV-2) in the presence of various amounts of human background DNA. **B.** Results of digital CRISPR reaction with target DNA and various amounts of human background DNA. Each point represents one sample. **C.** Comparison of the digital CRISPR reaction with or without 1ng/ $\mu$ L human background DNA.

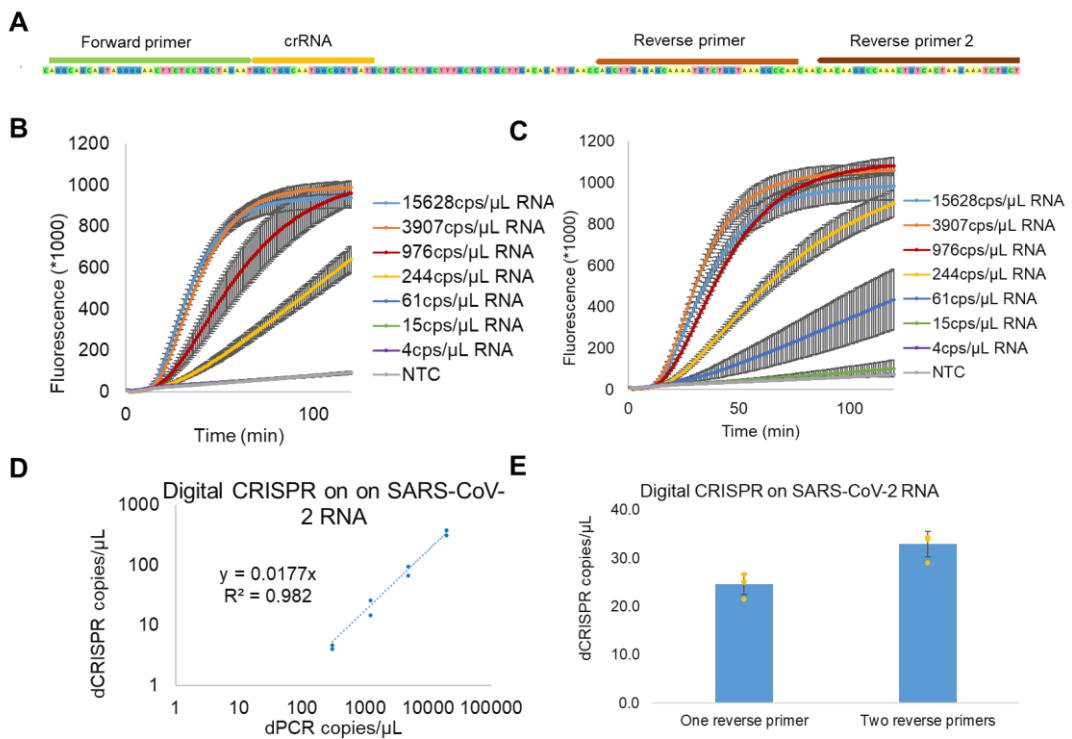

**Figure S6. Digital isothermal CRISPR reaction on RNA samples.** **A.** Design of two reverse primers to increase the sensitivity. **B, C.** Bulk RPA-Cas12a reaction on RNA at different concentrations with normal one reverse primer design (B) or two reverse primers design (C). **D.** Comparison of the absolute quantification result of digital isothermal CRISPR and digital PCR on SARS-CoV-2 RNA. **E.** Comparison of the digital CRISPR performance on normal one reverse primer design and two reverse primers design.

#### References:

1. Ding, X. et al. Ultrasensitive and visual detection of SARS-CoV-2 using all-in-one dual CRISPR-Cas12a assay. *Nature communications* **11**, 4711 (2020).
2. Qian, J. et al. An enhanced isothermal amplification assay for viral detection. *bioRxiv*, 2020.2005.2028.118059 (2020).