

1 Supplementary information

2 A Digital CRISPR-based Method for the Rapid Detection
3 and Absolute Quantification of Viral Nucleic Acids

4 Xiaolin Wu¹, Cheryl Chan¹, Yie Hou Lee¹, Stacy L. Springs^{1,2}, Timothy K.
5 Lu^{1,3,4,5,6,7,8*}, Hanry Yu^{1,9,10,11*}

6 ¹Singapore-MIT Alliance for Research and Technology, Critical Analytics for
7 Manufacturing of Personalized Medicine Interdisciplinary Research Group,
8 Singapore 138602, Singapore

9 ²Center for Biomedical Innovation, Massachusetts Institute of Technology,
10 Cambridge, MA, USA.

11 ³Synthetic Biology Center, Massachusetts Institute of Technology (MIT),
12 Cambridge, MA 02139, USA

13 ⁴Synthetic Biology Group, Research Laboratory of Electronics, Massachusetts
14 Institute of Technology (MIT), Cambridge, MA 02139, USA

15 ⁵Broad Institute of MIT and Harvard, Cambridge, MA 02142, USA

16 ⁶Department of Electrical Engineering and Computer Science, Massachusetts
17 Institute of Technology (MIT), Cambridge, MA 02142, USA

18 ⁷Harvard-MIT Division of Health Sciences and Technology, Cambridge, MA
19 02139, USA

20 ⁸Department of Biological Engineering, Massachusetts Institute of Technology
21 (MIT), Cambridge, MA 02142, USA

22 ⁹Institute of Bioengineering and Nanotechnology, A*STAR, The Nanos, #04-
23 01, 31 Biopolis Way, Singapore 138669, Singapore

24 ¹⁰Mechanobiology Institute, National University of Singapore, T-Lab, #05-01,
25 5A Engineering Drive 1, Singapore 117411, Singapore

26 ¹¹Department of Physiology, The Institute for Digital Medicine (WiSDM), Yong
27 Loo Lin School of Medicine, MD9-04-11, 2 Medical Drive, Singapore 117593,
28 Singapore

29 * Correspondence should be addressed to Timothy K. Lu (timlu@mit.edu) and
30 Hanry Yu (phsyuh@nus.edu.sg).

31 **Items included in supplementary information:**

32 **Supplementary Figures 1 to 6**

33 **Supplementary Tables 1 to 3**

34 **Supplementary References**

Supplementary Table 1. Primers and probes used in this study.

Name	Sequence	Application
ssDNA-FQ reporter	/56-FAM/TTATT/3IABkFQ/	Cas12a FQ reporter
N-RNA-F	gaaatTAATACGACTCACTATAgggATGTCTGA TAATGGACCCCAAAT	Amplify N gene on plasmid
N-RNA-R	gaaatTTAGGCCTGAGTTGAGTCAGCACT	Amplify N gene on plasmid
CHNCDC-geneN-F	GGGAACTTCTCCTGCTAGAAT	dPCR Primer for N gene
CHNCDC-geneN-R	CAGACATTTGCTCTCAAGCTG	dPCR Primer for N gene
CHNCDC-geneN-P	/56-FAM/TT GCT GCT G/ZEN/C TTG ACA GAT T/3IABkFQ/	dPCR Probe for N gene
T7-3G IVT primer	GAAATTAAATACGACTCACTATAAGGG	universal primer used for crRNA synthesis
N-N-RPA-F	AACTCCAGGCAGCAGTAGGGAACTT	CRISPR Primer for N gene
N-N-RPA-R	CCTTTACCAGACATTTGCTCTCAAG	CRISPR Primer for N gene
N-N-crRNA-IVT	AATCTGTCAAGCAGCAGATCTACACTTAGTA GAAATTACCTATAGTGAGTCGTATTAATTTC	crRNA template for N gene, pair with T7-3G IVT primer
N-AIOD-F ¹	AGGCAGCAGTAGGGAACTTCTCCTGCTAG AAT	RADICA Primer for N gene
N-AIOD-R ¹	TTGGCCTTACCAGACATTTGCTCTCAAGC TG	RADICA Primer for N gene
N-AIOD-crRNA-IVT-F	ggctggcaatggcggtatgATCTACACTTAGTAGAA ATTACCTATAGTGAGTCGTATTAATTTC	crRNA template for N gene, pair with T7-3G IVT primer
T7-Cas12scaffold-F	gaaatTAATACGACTCACTATAAGGTATTTCTA CTAAGTGTAGAT	universal primer used for crRNA synthesis
N-RPA-RR	AGCAGATTCTTAGTGACAGTTGGCCTTG TG	CRISPR Primer for N gene
N2-RPA-RR	AGCAAAATGACTTGATTTGAAATTGGAT CT	CRISPR Primer for N gene
N-JQ217-F ²	CAACTTCCTCAAGGAACAACATTGCCAAA	CRISPR Primer for N gene
N-JQ235-R ²	TGGAGTTGAATTCTTGAACTGTTGCGACT	CRISPR Primer for N gene
NF-CoV-RR	GAGAAGTTCCCCTACTGCTG	CRISPR Primer for N gene
NF-crRNA-1F	CTTCTACGCAGAAGGGAGCAatctacacttaga aatta	crRNA template for N gene, pair with T7-Cas12scaffold-F
EBV-EBNA1-F2	GCCGGTGTTCGTATATGGAGGTAGTAAG AC	RADICA Primer for EBV
EBV-EBNA1-R2	ATTCCAAAGGGAGACGACTCAATGGTGA A	RADICA Primer for EBV
EBNA-2R1-crRNAR	ACGACATTGTGGAAYAGCAAGGatctacacttagt agaaaatta	crRNA template for EBV, pair with T7-Cas12scaffold-F

36 **Supplementary Table 2. Quantification of linearized plasmid target by**
 37 **RADICA**

Number of replications	dPCR measured concentration (copies/µL)	Mean of RADICA measured concentration (copies/µL)	Standard deviation (copies/µL)	Relative standard deviation or coefficient of variation (CV)
10	Non template control	0.17	0.15	-
14	0.70	0.60	0.29	49.41%
14	2.80	2.20	0.25	11.25%
13	11.19	9.06	1.23	13.53%
14	44.76	35.53	5.30	14.91%
10	179.06	146.90	18.02	12.27%
10	716.24	626.58	73.96	11.80%
10	2387.46	2027.27	152.76	7.54%

38
39

40 **Supplementary Table 3. Comparison of RADICA with other viral detection**
 41 **methods.**

	RT-PCR	CRISPR-based isothermal method	RT-digital PCR	Digital RPA/digital LAMP	RADICA
Detecting Substance	RNA, DNA, cDNA	RNA, DNA, cDNA	RNA, DNA, cDNA	DNA, cDNA	DNA, cDNA
LoD (for SARS-CoV-2)	5 copies per reaction	20 copies per reaction	2 copies per reaction	NA	13.5 copies per reaction (0.897 copies/µL in 15 µL reaction)
Result Time	2 hours	1 hour	4 hours	1 hour	1 hour
Thermal cycling Requirements	Yes	No	Yes	No	No
All devices and regents commercially available	Yes	Yes	Yes	No	Yes
Ease of primer and crRNA design	Yes	Moderate	Yes	Moderate	Yes
Specificity	Good	Good	Good	Normal	Good
Absolute quantification	No	No	Yes	Yes	Yes

42 **Supplementary References**

- 43 1. Ding, X. et al. Ultrasensitive and visual detection of SARS-CoV-2 using
 44 all-in-one dual CRISPR-Cas12a assay. *Nature communications* **11**,
 45 4711 (2020).
- 46 2. Qian, J. et al. An enhanced isothermal amplification assay for viral
 47 detection. *bioRxiv*, 2020.2005.2028.118059 (2020).

48

49

Supplementary Figure 1. Cas12a detection sensitivity of dsDNA dilution series without pre-amplification. **a**, Kinetics of Cas12a-crRNA on dsDNA dilution series. **b**, Detection sensitivity analysis of dsDNA dilution series with Cas12a-crRNA in 1h. 50nM Cas12-crRNA and 250 nM FQ-ssDNA probe were incubated with dsDNA dilution series at 37°C and fluorescence was monitored every 5 min.

50


51

52

53

54

55

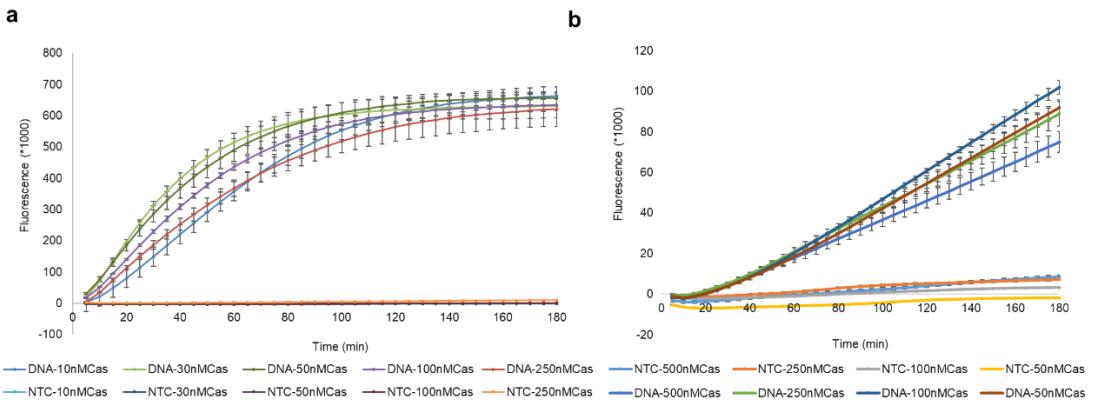


56

57 **Supplementary Figure 2. Detection of dsDNA without preamplification at**
 58 **different Cas12a/crRNA concentrations. a,** 1 nM dsDNA incubated with 10-
 59 250 nM Cas12a-crRNA and 250 nM FQ ssDNA probe. **b,** 0.1 nM dsDNA
 60 incubated with 50-500 nM Cas12a-crRNA and 500 nM FQ ssDNA probe.

61


62

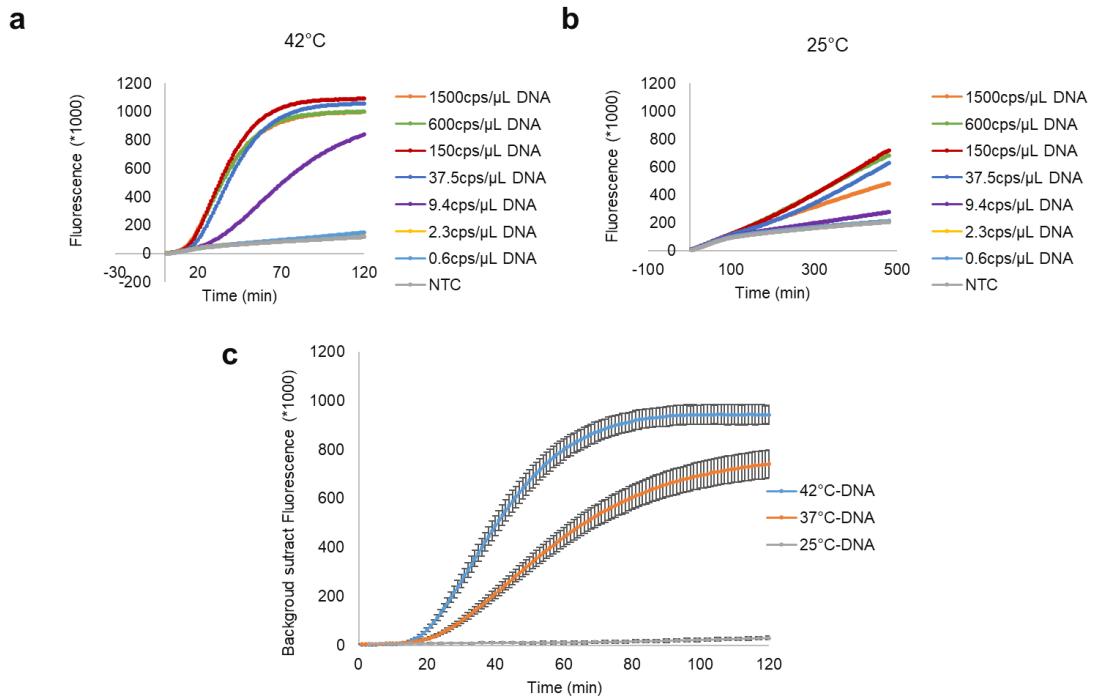

63

64 **Supplementary Figure 3. RPA+Cas12a bulk reaction at different**
 65 **temperatures.** **a, b,** RPA+Cas12a one-pot reaction on serial dilutions of DNA
 66 at 42°C **(a)** or 25°C **(b).** **c,** RPA+Cas12a one-pot reaction on 37.5 copies/μL
 67 plasmid DNA at different temperatures (25°C, 37°C, and 42°C).


68

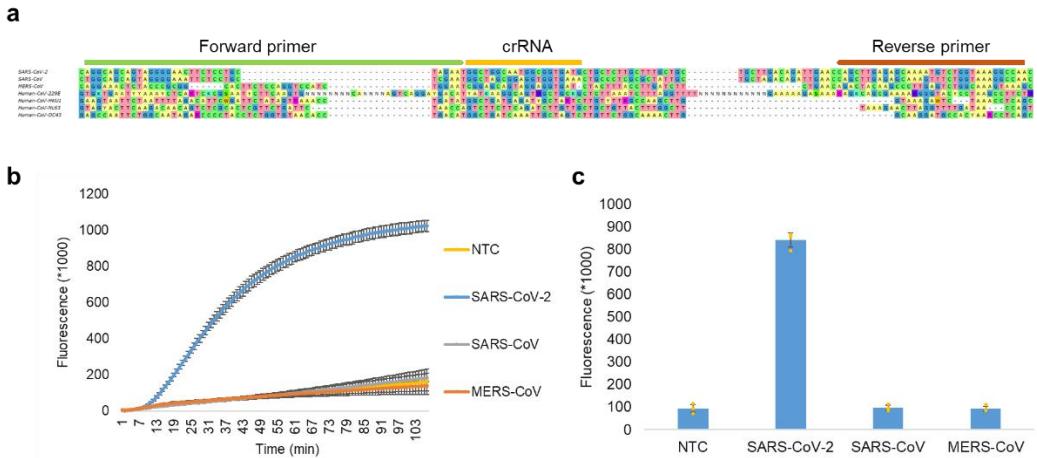

69

70 **Supplementary Figure 4. Specificity analysis for SARS-CoV-2.** **a**,
 71 Sequence alignment of the SARS-CoV-2 target region (N gene) and the
 72 corresponding regions on other human coronaviruses. **b**, Time course reaction
 73 of bulk RPA-Cas12a assay on SARS-CoV-2, SARS-CoV, and MERS-CoV N
 74 gene DNA target. The same concentration (25000 copies/ μ L) of the N gene
 75 target from different coronaviruses was tested by the bulk RPA-Cas12a assay.
 76 **c**, Specificity of the bulk RPA-Cas12a assay for detection of the SARS-CoV-2
 77 N gene.


78

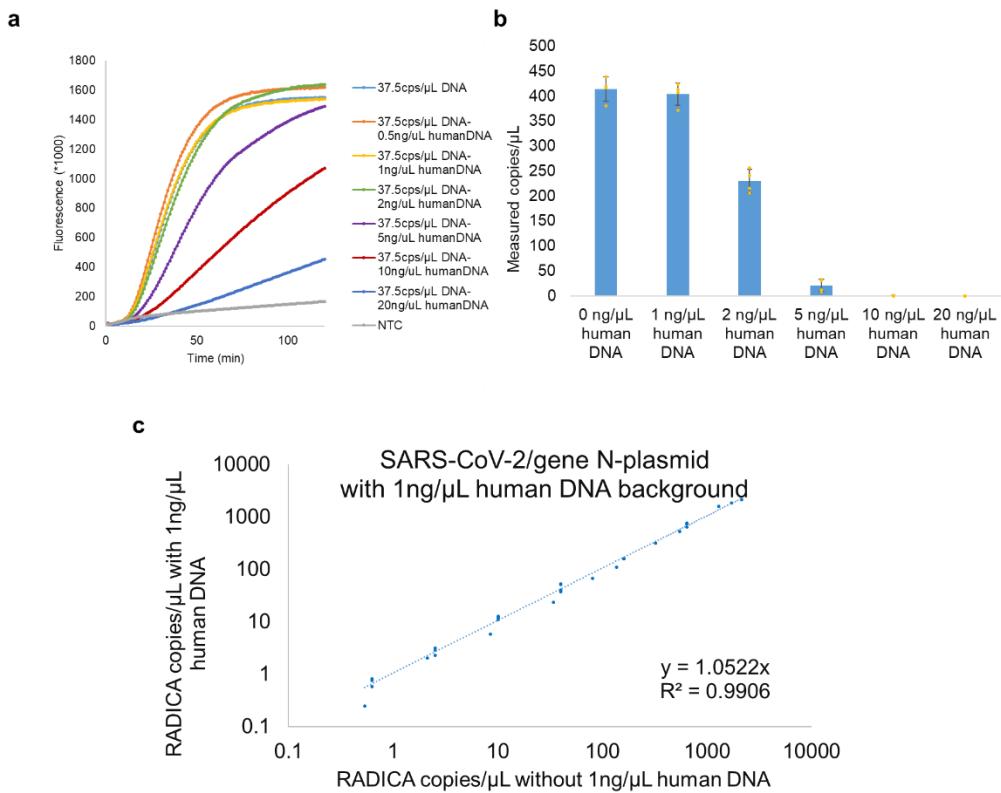

79

80 **Supplementary Figure 5. RPA inhibition by human background DNA.** **a,**
 81 Results of bulk RPA-Cas12a reaction to detect target DNA (i.e., the N gene
 82 from SARS-CoV-2) in the presence of various amounts of human background
 83 DNA. **b,** Results of RADICA reaction with target DNA and various amounts of
 84 human background DNA. Each point represents one sample. **c,** Comparison of
 85 the RADICA reaction with or without 1ng/μL human background DNA.

86

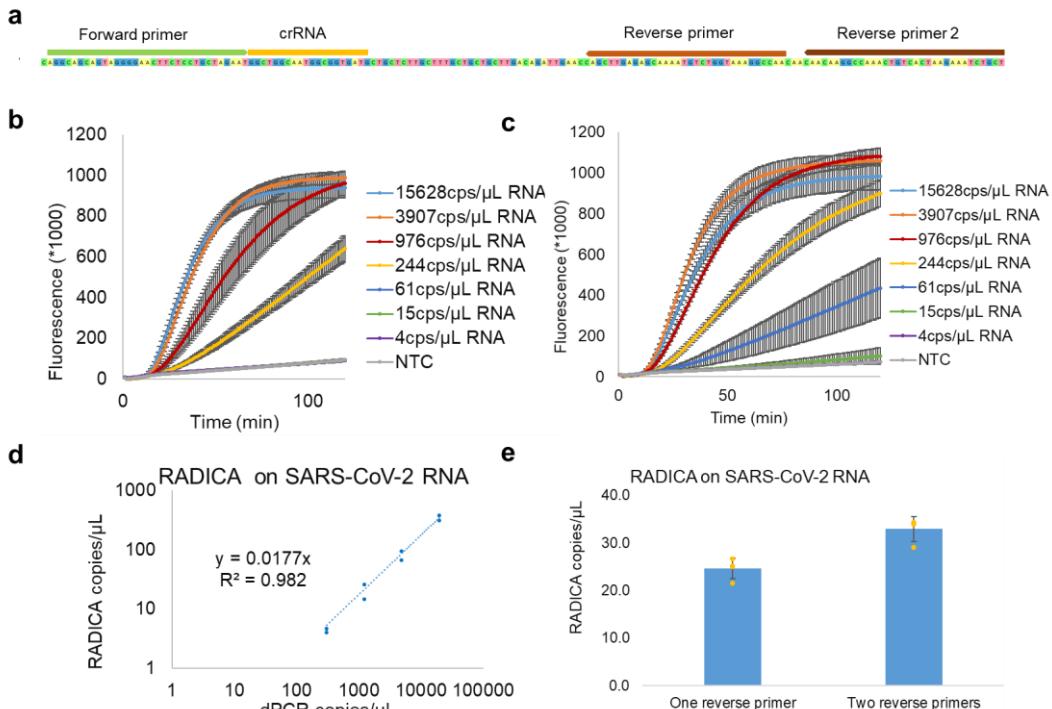

87

88 **Supplementary Figure 6. Digital isothermal CRISPR reaction on RNA**
 89 **samples.** **a**, Design of two reverse primers to increase the sensitivity. **b, c**, Bulk
 90 RPA-Cas12a reaction on RNA at different concentrations with normal one
 91 reverse primer design (**b**) or two reverse primers design (**c**). **d**, Comparison of
 92 the absolute quantification result of RADICA and digital PCR on SARS-CoV-2
 93 RNA. **e**, Comparison of RADICA's performance on normal one reverse primer
 94 design and two reverse primers design.

95