

**Supplementary Information:**

**An alternative approach for bioanalytical assay development for wastewater-based epidemiology of SARS-CoV-2**

Boogaerts Tim<sup>a,\*</sup>, De Roeck Naomi<sup>b</sup>, Jacobs Lotte<sup>b</sup>, van Nuijs L.N. Alexander<sup>a,\*\*</sup>, Delputte Peter<sup>b,\*\*</sup>

<sup>a</sup> Toxicological Centre, University of Antwerp, Universiteitsplein 1, 2610 Wilrijk, Belgium

<sup>b</sup> Laboratory for Microbiology, Parasitology and Hygiene, Universiteitsplein 1, 2610 Wilrijk, Belgium

\* - Corresponding author: [Tim.Boogaerts@uantwerpen.be](mailto:Tim.Boogaerts@uantwerpen.be)

\*\* - shared senior authors

## S.1. Sample preparation

### S.1.1. Standard operating procedures for the different sample concentration methods

#### Sample preparation Centricon 70 Plus, 100 kDa

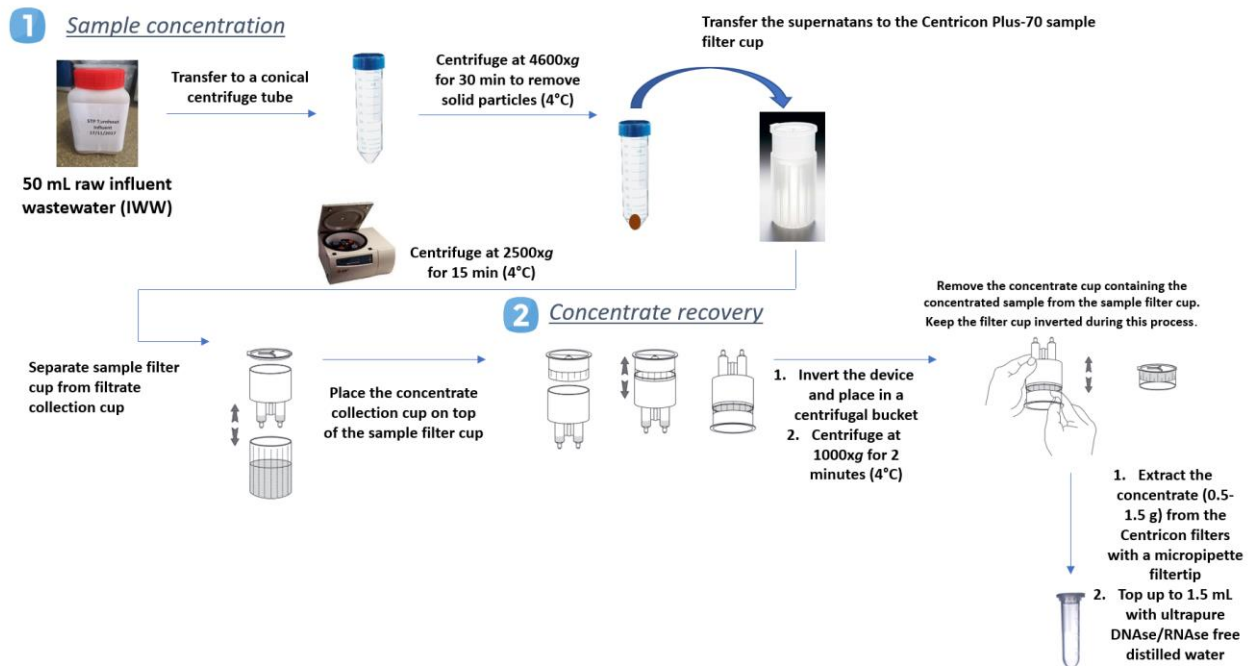


Figure S 1 SOP Centricon Plus-70 centrifugal devices

#### Sample preparation Vivaspin/Macrosep/Amicon 5-20 mL, 100 kDa

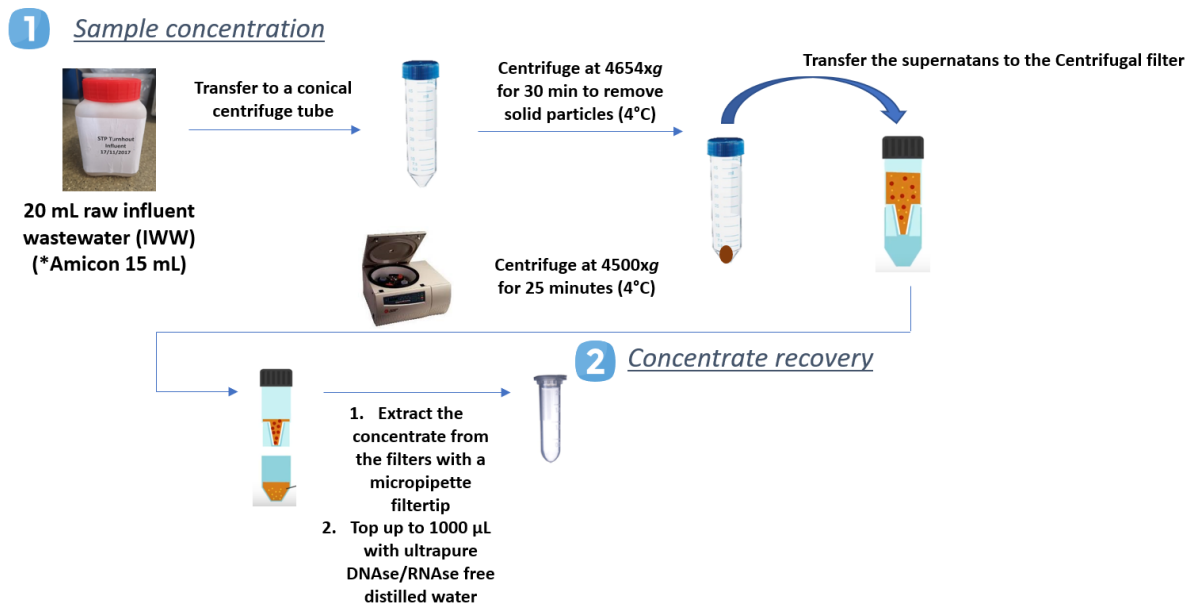


Figure S 2 SOP centrifugal filter units (Vivaspin/Macrosep/Amicon)

## Sample preparation PEG precipitation

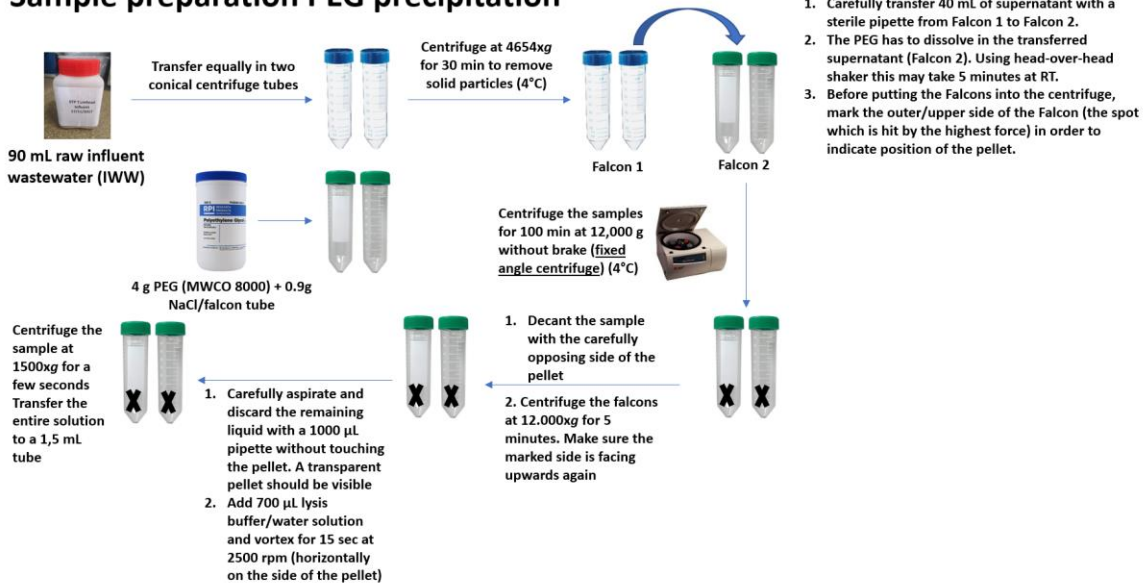


Figure S 3 SOP PEG precipitation

### S.1.2. Comparison of different sample preparation methods

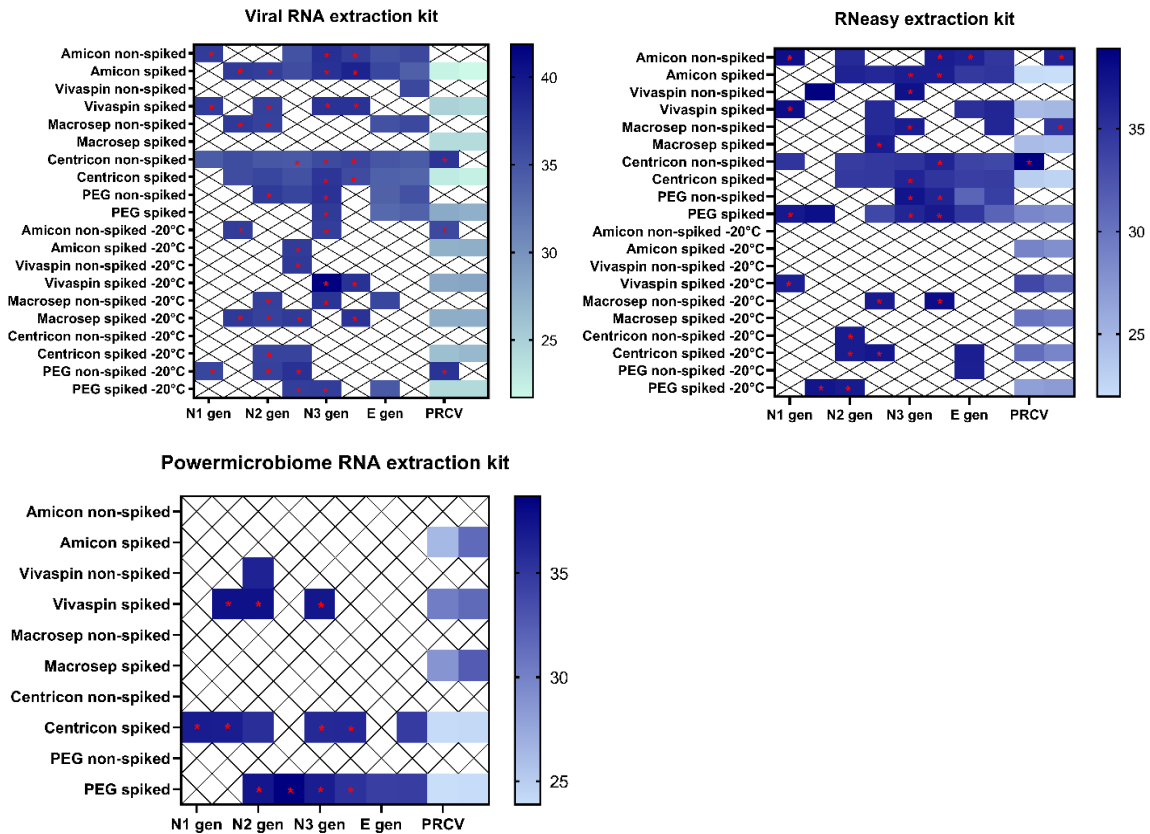


Figure S 4 Comparison of different sample concentration methods and RNA extraction kits with both frozen (-20°C) and fresh (4°C) IWW samples. The same sample was aliquoted in different fractions that were analyzed with the different sample concentration methods and RNA extraction kits.

## S. 1.2. Instrumental analysis

*Table S 1 Assessment of precision at different concentration levels with dPCR*

Calibration point	Target gene	Concentration (copies/ $\mu$ L)	Confidence interval (95%)	Number of valid partitions	Positive partition rate
10 <sup>4</sup>	N1	7967	1.0%	24882	76.6%
	N2	7212.5	1.1%	25426	73.1%
	E	6565.5	1.1%	25173	69.1%
10 <sup>3</sup>	N1	741	3.3%	25459	12.6%
	N2	665.5	3.5%	25469	11.4%
	E	591.5	3.7%	25451	10.2%
10 <sup>2</sup>	N1	70	10.9%	25453	1.2%
	N2	55.5	12.2%	25428	1.0%
	E	55	12.6%	24116	1.0%
10 <sup>1</sup>	N1	6	38.4%	24817	0.10%
	N2	7.5	33.6%	25460	0.13%
	E	6.5	36.3%	25451	0.11%
10 <sup>0</sup>	N1	1.505	79.0%	25468	0.027%
	N2	1.075	95.7%	25460	0.020%
	E	0	-	25439	0%
10 <sup>-1</sup>	N1	0	-	24753	0%
	N2	0.43	168,6%	25457	0.0079%
	E	0	-	25446	0%