


Supplementary Data:

Supplementary Figure and Table Legends:

Suppl. Figure 1: Relation of noise and MAPD quality values from all 102 PB samples analyzed with nanopore sequencing. MAPD: Median of the Absolute values of all Pairwise Differences; noise: median standard deviation of normalised read counts within each segment.

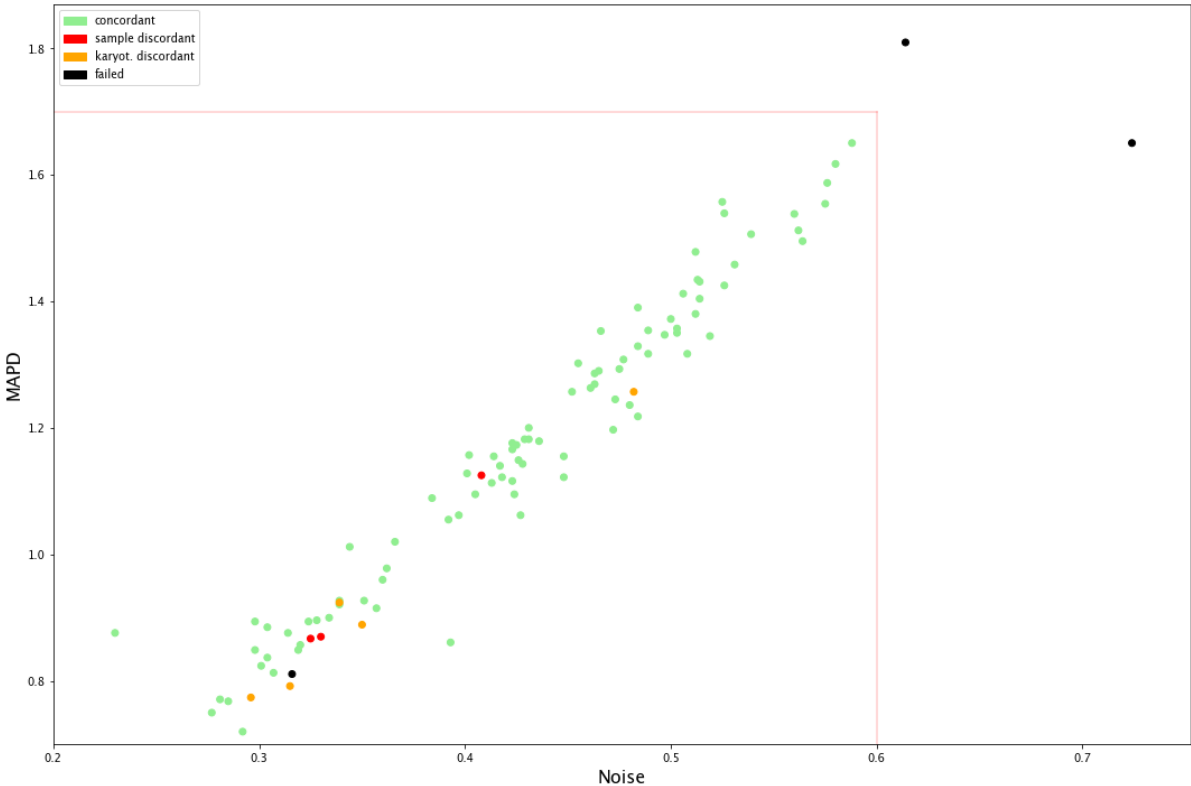

Suppl. Table 1: Detailed list of Nanopore sequencing results in comparison with aCGH results. All samples, that were digested with Endonuclease I after WGA are marked as EN.

Sample Number	Conc. after WGA (ng/μl)	Library Preparation		Nanopore Sequencing		Output			Ploidy Status			Chromosome Aberrations			manual evaluation of euploid nanopore results	
		Endonuclease digest	Barcode	Run	Time / Sample (min)	Yield (Mbases)	Raw Reads	noise	MAPD	aCGH	Nanopore	Concordance	aCGH	Nanopore		Concordance
Pb1	400	no	1	1	90	130	121.912	0.360	0.960	aneuploid	aneuploid	CONCORDANT	multiple (+2, -9, -15, -16)	multiple (+2, -9, -15, -16)	CONCORDANT	
Pb2	239	no	2	1	90	133	138.932	0.339	0.921	aneuploid	aneuploid	CONCORDANT	+22	-	CONCORDANT	
Pb3	283	no	3	1	90	104	94.894	0.304	0.885	euploid	euploid	CONCORDANT	-	-	CONCORDANT	ok
Pb4	264	no	4	1	90	111	104.648	0.314	0.876	euploid	euploid	CONCORDANT	-	-	CONCORDANT	ok
Pb5	447	no	5	2	70	115	104.473	0.392	1.053	aneuploid	aneuploid	CONCORDANT	-1	-1	CONCORDANT	ok
Pb6	347	yes	1	EN4	90	170	117.144	0.339	0.937	euploid	euploid	CONCORDANT	-	-	CONCORDANT	ok (+22)
Pb7	323	no	7	2	70	108	90.215	0.298	0.849	euploid	euploid	CONCORDANT	-	-	CONCORDANT	ok
Pb8	323	no	8	2	70	154	133.237	0.351	0.927	euploid	euploid	CONCORDANT	-	-	CONCORDANT	ok (+20)
Pb9	309	no	9	2	70	62	50.466	0.452	1.257	aneuploid	aneuploid	CONCORDANT	multiple (+7, +10, +20, +21, -22)	multiple (+7, +10, +21, -22)	CONCORDANT	
Pb10	303	yes	1	EN2	100	178	189.572	0.324	0.894	euploid	euploid	CONCORDANT	-	-	CONCORDANT	ok
Pb11	307	no	11	3	90	84	67.208	0.423	1.176	aneuploid	aneuploid	CONCORDANT	-4	-4	CONCORDANT	ok
Pb12	307	yes	2	EN2	100	245	274.533	0.281	0.771	euploid	euploid	CONCORDANT	-	-	CONCORDANT	ok
Pb13	302	no	3	3	90	64	48.057	0.466	1.353	aneuploid	aneuploid	CONCORDANT	-15	-15	CONCORDANT	ok
Pb14	299	yes	7	EN3	100	144	190.505	0.328	0.896	euploid	euploid	CONCORDANT	-	-	CONCORDANT	ok
Pb15	440	no	5	4	90	100	72.449	0.423	1.166	aneuploid	aneuploid	CONCORDANT	-10, +14	-10, +14	CONCORDANT	
Pb16	460	no	6	4	90	104	75.678	0.415	1.155	aneuploid	aneuploid	CONCORDANT	+10, +X	+10, +X	CONCORDANT	
Pb17	460	no	7	4	90	64	53.288	0.473	1.245	aneuploid	aneuploid	CONCORDANT	-14, +20	-14, +20	CONCORDANT	
Pb18	387	yes	3	EN2	100	142	172.952	0.344	1.022	aneuploid	aneuploid	CONCORDANT	multiple (+1, +4, -5, +17, -21, +22)	multiple (+1, +4, -5, +17, -21, +22)	CONCORDANT	
Pb19	400	no	9	4	90	60	46.297	0.514	1.404	aneuploid	aneuploid	CONCORDANT	+16, -18, -20	+16, -18, -20	CONCORDANT	
Pb20	453	yes	8	EN3	100	176	233.128	0.482	1.257	aneuploid	aneuploid	CONCORDANT	-7, +16	multiple (-7, +9, +10, +16, +17)	DISCORDANT	
Pb21	281	yes	9	EN3	100	148	197.323	0.339	0.924	aneuploid	aneuploid	CONCORDANT	+19, -21, -22	-21	DISCORDANT	
Pb22	340	no	2	5	120	112	97.165	0.425	1.173	aneuploid	aneuploid	CONCORDANT	+12, -13, -16	-	CONCORDANT	
Pb23	353	no	3	5	120	99	82.572	0.405	1.095	euploid	euploid	CONCORDANT	-	-	CONCORDANT	ok
Pb24	300	no	4	5	120	112	92.960	0.426	1.149	euploid	euploid	CONCORDANT	-	-	CONCORDANT	ok
Pb25	258	yes	1	EN1	120	211	231.486	0.319	0.849	euploid	euploid	CONCORDANT	-	-	CONCORDANT	ok
Pb26	223	yes	2	EN1	120	281	361.988	0.277	0.750	aneuploid	aneuploid	CONCORDANT	-16	-16	CONCORDANT	ok
Pb27	295	yes	3	EN1	120	227	268.410	0.285	0.768	euploid	euploid	CONCORDANT	-	-	CONCORDANT	ok
Pb28	325	yes	4	EN1	120	253	311.201	0.292	0.720	aneuploid	aneuploid	CONCORDANT	-6, -12	-6, -12	CONCORDANT	
Pb29	309	yes	4	EN5	90	183	222.899	0.307	0.813	euploid	euploid	CONCORDANT	-	-	CONCORDANT	ok
Pb30	331	yes	10	EN3	100	155	220.552	0.230	0.876	aneuploid	aneuploid	CONCORDANT	+11, +15, +22	+11, +15, +22	CONCORDANT	
Pb31	333	no	1	7	70	106	75.428	0.384	1.089	aneuploid	aneuploid	CONCORDANT	-17	-17	CONCORDANT	
Pb32	413	yes	4	EN2	100	189	218.267	0.298	0.894	aneuploid	aneuploid	CONCORDANT	multiple (+3, +11, +12, +16, +19)	multiple (+3, +4, +11, +12, +16, +19)	CONCORDANT	
Pb33	413	yes	11	EN3	100	174	243.733	0.320	0.857	aneuploid	aneuploid	CONCORDANT	multiple (+2, +9, -15, +19)	multiple (+2, +9, -15, +19)	CONCORDANT	
Pb34	367	yes	12	EN3	100	132	208.681	0.301	0.824	aneuploid	aneuploid	CONCORDANT	-13, -15, -21	-13, -15, -21	CONCORDANT	
Pb35	331	no	5	7	70	128	91.228	0.362	0.978	aneuploid	aneuploid	CONCORDANT	-22	-22	CONCORDANT	
Pb36	360	no	6	8	70	108	83.115	0.366	1.020	euploid	euploid	CONCORDANT	-	-	CONCORDANT	ok (+19)
Pb37	333	no	7	8	70	94	69.548	0.489	1.317	aneuploid	aneuploid	CONCORDANT	+16	+16	CONCORDANT	
Pb38	300	yes	8	EN5	90	190	246.494	0.448	1.122	euploid	euploid	CONCORDANT	-	-	CONCORDANT	ok (+22)
Pb39	347	no	9	8	70	71	54.614	0.428	1.143	aneuploid	aneuploid	CONCORDANT	multiple (-7, +16, -18, -22)	multiple (-7, +16, -18, -22)	CONCORDANT	
Pb40	373	no	10	8	70	81	58.109	0.417	1.140	aneuploid	aneuploid	CONCORDANT	+4	+4	CONCORDANT	
Pb41	297	no	11	8	70	92	68.813	0.393	0.861	aneuploid	aneuploid	CONCORDANT	multiple (+3, -6, -7, -8, -9, -10, -12, +13, +14, -17, -18, -19, -21)	multiple (+3, -6, -7, -8, -9, -10, -12, +13, +14, -17, -18, -19, -21)	CONCORDANT	
Pb42	353	no	1	9	90	95	65.990	0.513	1.434	aneuploid	aneuploid	CONCORDANT	multiple (+1, +4, +8, +10, +11, +12, +13, +14, -15, +16, +18, +21, +22)	multiple (+1, +4, +8, +10, +11, +12, +14, -15, +16, +18, +21, +22)	CONCORDANT	
Pb43	353	no	2	9	90	90	59.374	0.424	1.095	aneuploid	aneuploid	CONCORDANT	multiple (-4, -7, -8, -10, -12, -13, -17, +19, -20, -21, +22, +X)	multiple (-4, -7, -8, -10, -12, -13, -16, -17, -20, -21)	CONCORDANT	
Pb44	433	no	3	9	90	73	51.420	0.455	1.302	aneuploid	aneuploid	CONCORDANT	+15	+15	CONCORDANT	
Pb45	347	no	4	9	90	102	68.937	0.401	1.128	aneuploid	aneuploid	CONCORDANT	+16, -19	+16, -19	CONCORDANT	
Pb46	347	no	5	9	90	100	70.807	0.408	1.125	aneuploid	aneuploid	DISCORDANT	+22	-	DISCORDANT	ok (+22)
Pb47	380	no	6	9	90	90	70.894	0.402	1.157	aneuploid	aneuploid	CONCORDANT	multiple (+10, -14, +16, +18)	multiple (+10, -14, +16, +18)	CONCORDANT	
Pb48	323	no	7	10	80	35	22.063	0.614	1.890	euploid	not evaluable	EXCLUDED	-	-	EXCLUDED	
Pb49	330	no	8	10	80	47	31.641	0.512	1.380	euploid	euploid	CONCORDANT	-	-	CONCORDANT	ok
Pb50	360	no	9	10	80	45	33.090	0.580	1.617	euploid	euploid	CONCORDANT	-	-	CONCORDANT	ok
Pb51	329	no	10	10	80	46	32.845	0.531	1.458	aneuploid	aneuploid	CONCORDANT	multiple (-7, -9, +16, -19)	multiple (-7, -9, +16, -19)	CONCORDANT	
Pb52	321	no	11	10	80	52	37.722	0.480	1.236	euploid	euploid	CONCORDANT	-	-	CONCORDANT	ok
Pb53	380	no	12	10	80	58	43.439	0.576	1.587	euploid	euploid	CONCORDANT	-	-	CONCORDANT	ok
Pb54	302	no	1	11	80	54	45.582	0.477	1.308	aneuploid	aneuploid	CONCORDANT	-9, -15	-9, -15	CONCORDANT	
Pb55	413	no	2	11	80	51	39.452	0.484	1.329	aneuploid	aneuploid	CONCORDANT	-17, -18	-17, -18	CONCORDANT	
Pb56	367	no	3	11	80	51	42.753	0.526	1.425	aneuploid	aneuploid	CONCORDANT	-16	-16	CONCORDANT	
Pb57	380	no	4	11	80	62	48.039	0.463	1.269	euploid	euploid	CONCORDANT	-	-	CONCORDANT	ok (+16)
Pb58	353	yes	2	EN4	90	152	96.024	0.350	0.889	aneuploid	aneuploid	CONCORDANT	-13, -14, +17	multiple (+11, -13, -14, +15, +17, +21)	DISCORDANT	
Pb59	360	no	6	11	80	40	30.948	0.526	1.539	aneuploid	aneuploid	CONCORDANT	multiple (+3, +9, -13, +17, -18, -X)	multiple (+3, +9, -13, +17, -18, -X)	CONCORDANT	
Pb60	311	no	12	12	77	130	35.414	0.512	1.478	euploid	euploid	CONCORDANT	-	-	CONCORDANT	ok
Pb61	228	no	1	12	77	180	50.758	0.724	1.650	not evaluable	euploid	EXCLUDED	-	-	EXCLUDED	
Pb62	340	yes	9	EN5	90	270	171.404	0.325	0.867	aneuploid	aneuploid	DISCORDANT	+19	-	DISCORDANT	ok (+19)
Pb63	373	no	3	12	77	180	74.607	0.508	1.317	aneuploid	aneuploid	CONCORDANT	multiple (+5, -11, +15, +17, +19)	multiple (+5, -11, +15, +17(s), +19)	CONCORDANT	
Pb64	319	no	4	12	77	230	57.518	0.413	1.113	aneuploid	aneuploid	CONCORDANT	+4	+4	CONCORDANT	
Pb65	387	no	5	12	77	180	47.973	0.461	1.263	aneuploid	aneuploid	CONCORDANT	+16	+16	CONCORDANT	
Pb66	254	no	6	12	77	200	56.133	0.506	1.412	aneuploid	aneuploid	CONCORDANT	multiple (-9, +10, +11, -13, -16, -18, -20, +21, +22)	multiple (+11, -13, -16, -18, -20, +22)	CONCORDANT	
Pb67	371	no	1	13	80	56	35.184	0.500	1.372	aneuploid	aneuploid	CONCORDANT	+12, -15	+12, -15	CONCORDANT	
Pb68	301	no	2	13	80	77	47.042	0.431	1.200	aneuploid	aneuploid	CONCORDANT	+2	+2	CONCORDANT	
Pb69	356	no	3	13	80	50	30.943	0.560	1.538	aneuploid	aneuploid	CONCORDANT	+6, -18	+6, -18	CONCORDANT	
Pb70	294	no	4	13	80	71	46.296	0.431	1.182	aneuploid	aneuploid	CONCORDANT	-16, -22	-16, -22	CONCORDANT	
Pb71	353	no	5	13	80	63	43.959	0.465	1.290	aneuploid	aneuploid	CONCORDANT	+11, +16, -17	+11, +16, -17	CONCORDANT	
Pb72	445	no	6	13	80	75	53.594	0.484	1.218	aneuploid	aneuploid	CONCORDANT	-19	-19	CONCORDANT	
Pb73	510	no	7	14	90	53	33.809	0.484	1.390	aneuploid	aneuploid	CONCORDANT	+4, -20	+4, -20	CONCORDANT	
Pb74	474	yes	10	EN5	90	149</										

Suppl. Table 2: Calculation of time and cost of Nanopore sequencing workflow for polar body PGT-A.

Step	Material	Cost/sample for 1 sample	Cost/sample for 12 samples	Time for 1 sample	Time for 12 samples
WGA	PicoPlex WGA Kit	48 €	26 €	2,5 h	2,5 h
	OR:	OR	OR	OR	OR
in our study:	<u>REPLlg Single Cell Kit</u> incl. Endonuclease I digest	<u>54 €</u>	<u>30 €</u>	<u>2.5 h</u>	<u>3.5 h</u>
	OR:	OR	OR	OR	OR
	REPLlg Ultra Fast Mini Kit Incl. Endonuclease I digest	26 €	14 €	1,5 h	2,5 h
CAVE: One negative control is included in each WGA run to detect contamination and will not be handled further.					
Library Prep	details see Suppl. Table 3	70€	45€	1 h	2 x 5 h
Sequencing (and Basecalling)	Flow Cell (min. 48 Flow cells/year) → calculated if flow cell is re-used 5x for one sample each	95€	40€	30 min	2 x 6 h
Data analysis	PC/NAS/Server			5 min	30-60 min
TOTAL (dependent on WGA Kit)		190€ - 220€	100€ - 120€	3 h – 5 h	14 h – 16 h

Suppl. Table 3: Detailed list of costs for consumable material for nanopore sequencing workflow. All prices were obtained in December 2022 from the respective supplier websites with Austrian-based settings.

WGA:

- PicoPlex WGA Kit (Takara #R30050, 50 rx) 1188€ 23,76€/sample

OR:

- REPLI-g Ultra Fast Mini Kit (QIAGEN #150035, 100 rx) 901€ 9€/sample
- OR: REPLI-g Single Cell Kit (QIAGEN #150345, 96rx) 2202€ 23€/sample
- NEB T7 Endonuclease I (NEB, #M0302L) 293€ 4,20€/sample

Library Prep:

- NEBNext Ultra II End Prep/dA Tailing Module (NEB #E7546L, 96rx) 835€ 8,70€/sample
- NEBNext FFPE DNA Repair Mix (NEB, #M6630L, 96rx) 604€ 6,30€/sample
- gDNA Clean & Concentrator-25 (Zymo #D4065, 100rx) 329€ 3,29€/ sample
- 2x DNA Clean & Concentrator-5 (Zymo #D4004, 200rx) 299€ 2,99€/ sample
- Elution Buffer (QIAGEN, #19086, 250 ml) 35€ 0,50€/ sample
- Blunt/TA Ligase Master Mix (NEB #M0367, 50rx) 370€ 7,40€/ sample
- Quick T4 DNA Ligase (NEB #M2200L, 15 Libraries) 396€ 26€/library
- Native barcoding kit (ONT, EXP-NBD104, 12 BC) 259€ 3,60€/ sample
- Ligation Sequencing Expansions (instead of SQK-LSK109) (ONT, SFB001, AUX001, AMII001, each 12rx) 359€ ca. 4€/ sample
- Flow Cell Priming Kit (ONT, EXP-FLP002) 35€ ca. 1€/ sample
- Flow Cell Wash Kit (ONT, WSH004) 90€ ca. 2€/ sample

Quality control:

- Agarose E-Gel 2% (Thermo, #A42135, 10 Gels) 120€ 1,50€/ sample
- 3x Qubit BR Assay (Thermo, #Q32853, 500rx) 327€ 2€/ sample

For one sample: 70€ / sample

For 12 samples: 45 € / sample

Suppl. Table 4: Outcome measures of nanopore sequencing samples with and without Endonuclease I digestion step.

Sample	Run		Time / Sample (min)		Yield [Mb]		Raw Reads		noise		MAPD		Ploidy Status					Chromosome aberrations				
Sample Number	Without EN	With EN	Without EN	With EN	Without EN	With EN	Without EN	With EN	Without EN	With EN	Without EN	With EN	aCGH	Nanopore	Nanopore with EN	Concordance without EN	Concordance with EN	aCGH	Nanopore	Nanopore with EN	Concordance without EN	Concordance with EN
Pb25	6	EN1	96	120	102	211	77.207	231.486	0,369	0,319	0,963	0,849	euploid	euploid	euploid	CONCORDANT	CONCORDANT	-	-	-	CONCORDANT	CONCORDANT
Pb26	6	EN1	96	120	118	281	87.497	361.988	0,378	0,277	1,033	0,75	aneuploid	aneuploid	aneuploid	CONCORDANT	CONCORDANT	-16	-16	-16	CONCORDANT	CONCORDANT
Pb27	6	EN1	96	120	101	227	71.566	268.420	0,402	0,285	1,152	0,768	euploid	euploid	euploid	CONCORDANT	CONCORDANT	-	-	-	CONCORDANT	CONCORDANT
Pb28	6	EN1	96	120	109	253	86.791	311.201	0,395	0,292	1,047	0,72	aneuploid	aneuploid	aneuploid	CONCORDANT	CONCORDANT	-6, -12	-6, -12	-6, -12	CONCORDANT	CONCORDANT
Pb10	3	EN2	70	100	67	178	59.844	189.572	0,431	0,324	1,201	0,894	euploid	euploid	euploid	CONCORDANT	CONCORDANT	-	-	-	CONCORDANT	CONCORDANT
Pb12	3	EN2	90	100	58	245	46.745	274.533	0,394	0,281	1,149	0,771	euploid	euploid	euploid	CONCORDANT	CONCORDANT	-	-	-	CONCORDANT	CONCORDANT
Pb18	4	EN2	90	100	195	142	164.091	172.952	0,351	0,344	0,950	1,012	aneuploid	aneuploid	aneuploid	CONCORDANT	CONCORDANT	multiple	multiple	multiple	CONCORDANT	CONCORDANT
Pb32	7	EN2	70	100	109	189	83.677	218.267	0,397	0,298	1,134	0,894	aneuploid	aneuploid	aneuploid	CONCORDANT	CONCORDANT	multiple	multiple	multiple	CONCORDANT	CONCORDANT
Pb86	16	EN2	100	100	101	261	67.671	330.514	0,500	0,427	1,244	1,062	aneuploid	aneuploid	aneuploid	CONCORDANT	CONCORDANT	multiple	multiple	multiple	CONCORDANT	CONCORDANT
Pb87	16	EN2	100	100	49	158	34.733	185.739	0,516	0,334	1,479	0,900	aneuploid	aneuploid	aneuploid	CONCORDANT	CONCORDANT	+20	+20	+20	CONCORDANT	CONCORDANT
Pb14	3	EN3	90	100	68	144	54.967	190.505	0,449	0,328	1,272	0,896	euploid	euploid	euploid	CONCORDANT	CONCORDANT	-	-	-	CONCORDANT	CONCORDANT
Pb20	4	EN3	90	100	105	176	92.290	233.128	0,537	0,482	1,389	1,257	aneuploid	aneuploid	aneuploid	CONCORDANT	CONCORDANT	-7, +16	multiple	multiple	DISCORDANT	DISCORDANT
Pb21	5	EN3	120	100	92	148	74.701	197.323	0,388	0,339	1,074	0,924	aneuploid	aneuploid	aneuploid	CONCORDANT	CONCORDANT	+19, -21, -22	-21	-21	DISCORDANT	DISCORDANT
Pb30	7	EN3	70	100	96	155	69.559	220.552	0,390	0,320	1,104	0,876	aneuploid	aneuploid	aneuploid	CONCORDANT	CONCORDANT	+11, +15, +22	+11, +15	+11, +15, +22	DISCORDANT	CONCORDANT
Pb33	7	EN3	70	100	86	174	62.702	243.733	0,427	0,320	1,140	0,857	aneuploid	aneuploid	aneuploid	CONCORDANT	CONCORDANT	multiple	-2, +9, -15	+2, +9, -15	DISCORDANT	DISCORDANT
Pb34	7	EN3	70	100	106	132	78.244	208.681	0,378	0,301	1,047	0,824	aneuploid	aneuploid	aneuploid	CONCORDANT	CONCORDANT	-13, -15, -21	-13, -15	-13, -15, -21	DISCORDANT	CONCORDANT
Pb6	2	EN4	70	90	86	170	79.915	117.144	0,337	0,339	1,005	0,927	euploid	euploid	euploid	CONCORDANT	CONCORDANT	-	-	-	CONCORDANT	CONCORDANT
Pb58	11	EN4	80	90	79	152	65.709	96.024	0,398	0,350	1,041	0,889	aneuploid	aneuploid	aneuploid	CONCORDANT	CONCORDANT	-13, -14, +17	multiple	multiple	DISCORDANT	DISCORDANT
Pb78	14	EN4	90	90	72	115	48.876	73.728	0,503	0,423	1,368	1,116	aneuploid	aneuploid	aneuploid	CONCORDANT	CONCORDANT	+17, -22	+17	+17, -22	DISCORDANT	CONCORDANT
Pb91	17	EN4	80	90	28	28	21.405	92.844	0,630	0,357	1,671	0,915	aneuploid	aneuploid	aneuploid	CONCORDANT	CONCORDANT	-2, +6	-2, -21	-2, +6	DISCORDANT	CONCORDANT
Pb93	17	EN4	80	90	47	47	44.624	181.363	0,442	0,315	1,173	0,792	aneuploid	aneuploid	aneuploid	CONCORDANT	CONCORDANT	+1, -16, +19	+1, -16	+1, -16	DISCORDANT	DISCORDANT
Pb96	17	EN4	80	90	66	158	60.677	138.336	0,389	0,296	1,017	0,774	aneuploid	aneuploid	aneuploid	CONCORDANT	CONCORDANT	+11, -16, +19	+11, -16	+11, -16	DISCORDANT	DISCORDANT
Pb29	6	EN5	96	90	98	183	77.560	222.899	0,403	0,307	1,082	0,813	euploid	euploid	euploid	CONCORDANT	CONCORDANT	-	-	-	CONCORDANT	CONCORDANT
Pb38	8	EN5	70	90	110	190	82.209	246.494	0,506	0,448	1,266	1,122	euploid	aneuploid	euploid	DISCORDANT	CONCORDANT	-	-17	-	DISCORDANT	CONCORDANT
Pb62	12	EN5	77	90	180	136	51.856	171.404	0,441	0,325	1,155	0,867	aneuploid	euploid	euploid	DISCORDANT	DISCORDANT	+19	-	-	DISCORDANT	DISCORDANT
Pb74	14	EN5	90	90	76	149	48.009	214.091	0,447	0,304	1,233	0,837	aneuploid	euploid	aneuploid	DISCORDANT	CONCORDANT	-16, +21	-	-16, +21	DISCORDANT	CONCORDANT
Pb85	16	EN5	100	90	61	155	42.281	246.406	0,482	0,330	1,305	0,870	aneuploid	euploid	euploid	DISCORDANT	DISCORDANT	-16	-	-	DISCORDANT	DISCORDANT
Pb95	17	EN5	80	90	50	124	44.210	187.577	0,440	0,316	1,179	0,811	not evaluable	euploid	euploid	EXCLUDED	EXCLUDED	not evaluable	-	-	EXCLUDED	EXCLUDED