

Appendix

SUPPLEMENTAL TABLES

Table S1	Definitions of outcomes in health records
Table S2	GWAS summary statistics data source
Table S3	Multivariable Mendelian randomization (MVMR) analysis results for association of body mass index (BMI) with heart failure (HF)
Table S4	Mendelian Randomization Pleiotropy RESidual Sum and Outlier (MR-PRESSO) analysis results for association of body mass index (BMI) with heart failure (HF)
Table S5	Univariate Mendelian randomization (MR) analysis results for association of BMI with heart failure outcome adjusted using mtCoJo at summary statistics

Table S1. Definitions of outcomes in health records

Trait	ICD9 (ONS)	ICD10 (ONS)	ICD10 (HES)	OPCS4 (HES)	Read (CPRD)	Medications (BNF)
Heart failure	4151, 428	I11.0, I13.0, I13.2, I26.0, I50	I50.0, I50.1, I50.9, I11.0, I13.0, I32.2		G580400,G210.00,G210000,G210100,G211100, G21z100,G230.00,G232.00,G234.00,G1yz100, I01..00,662W.00,662p.00,8B29.00,8H2S.00, 9Or0.00,G400.00,G41z.11,G554000,G554011, G58..00,G58..11,G580.00,G580.11,G580.12, G580.13,G580.14,G580000,G580100,G580200, G580300,G581.00,G581.11,G581.13,G581000, G582.00,G58z.00,G58z.12,G5yy900,G5yyA00, R2y1000,Q48y100,585f.00,585g.00	
Coronary artery disease	-	-	I200, I201, I208, I209, I21, I22, I23, I240, I241, I248, I249, I25, I252	K40,K40.1,K40.2,K40.3,K40.4,K40.8,K40.9,K41,K4 1.1,K41.2,K41.3,K41.4,K41.8,K41.9,K42,K42.1,K42 .2,K42.3,K42.4,K42.8,K42.9,K43,K43.1,K43.2,K43. 3,K43.4,K43.8,K43.9,K44,K44.1,K44.2,K44.8,K44.9 ,K45,K45.1,K45.2,K45.3,K45.4,K45.5,K45.6,K45.8, K45.9,K46,K46.1,K46.2,K46.3,K46.4,K46.5,K46.8, K46.9	1822,1823,1824,1825,1826,1827,1827.11,1828,1829,3233,3234,3235,3236,182..00,182A.00, 182B.00,182B000,182C.00,182Z.00,323..00,323Z.00,889A.00,8HTG.00,8HTJ.00,9Nof.00,G 30..00,G30..12,G30..13,G30..15,G30..16,G300.00,G301.00,G301000,G301100,G301z00,G3 02.00,G303.00,G304.00,G305.00,G306.00,G307.00,G307000,G307100,G308.00,G309.00,G 30B.00,G30X.00,G30X000,G30y.00,G30y000,G30y100,G30y200,G30yz00,G30z.00,G31y1 00,G33z400,G38..00,G380.00,G381.00,G384.00,G38z.00,Gyu3400,R065.00,R065000,R065 011,R065100,R065200,R065300,R065400,R065500,R065600,R065700,R065800,R065900, R065A00,R065B00,R065B14,R065C00,R065D00,R065z00,Ryu0400	2.6.1,2.6.3
Atrial fibrillation	-	-	I48	K01,K011,K012,K018,K019,K02,K021,K022,K023, K024,K025,K026,K028,K029,K04,K041,K042,K043 ,K044,K045,K046,K048,K049,K05,K051,K052,K05 8,K059,K06,K061,K062,K063,K064,K068,K069,K0 7,K071,K072,K073,K078,K079,K08,K081,K082,K0 83,K084,K088,K089,K09,K091,K092,K093,K094,K 095,K096,K098,K099,K10,K101,K102,K103,K104, K105,K108,K109,K11,K111,K112,K113,K114,K115 ,K116,K117,K118,K119,K12,K121,K122,K123,K12 4,K125,K128,K129,K14,K141,K142,K143,K144,K1 45,K148,K149,K15,K151,K152,K158,K159,K17,K1 71,K172,K173,K174,K175,K176,K177,K178,K179, K18,K181,K182,K183,K184,K185,K186,K187,K188 ,K189,K19,K191,K192,K193,K194,K195,K196,K19 8,K199,K20,K201,K202,K203,K204,K208,K209,K2 2,K221,K222,K228,K229,K23,K231,K232,K233,K2 34,K235,K236,K238,K239,K24,K241,K242,K243,K 244,K245,K246,K247,K248,K249,K25,K251,K252, K253,K254,K255,K258,K259,K26,K261,K262,K263 ,K264,K265,K268,K269,K27,K271,K272,K273,K27 4,K275,K276,K278,K279,K28,K281,K282,K283,K2 84,K285,K288,K289,K29,K291,K292,K293,K294,K 295,K296,K297,K298,K299,K30,K301,K302,K303, K304,K305,K308,K309,K31,K311,K312,K313,K314 ,K315,K318,K319,K32,K321,K322,K323,K324,K32 8,K329,K33,K331,K332,K333,K334,K335,K336,K3 38,K339,K34,K341,K342,K343,K344,K345,K346,K 348,K349,K36,K361,K362,K368,K369,K37,K371,K 372,K373,K374,K375,K376,K378,K379,K38,K381, K382,K383,K384,K385,K386,K388,K389,K40,K401 ,K402,K403,K404,K408,K409,K41,K411,K412,K41 3,K414,K418,K419,K42,K421,K422,K423,K424,K4 28,K429,K43,K431,K432,K433,K434,K438,K439,K 44,K441,K442,K448,K449,K45,K451,K452,K453,K 454,K455,K456,K458,K459,K46,K461,K462,K463,	3272,3273,7900,7901,7902,7902.11,7903,7903.11,7903.12,7903.13,7904,7905,7906,7906.11 ,7907,7907.11,7908,7908.11,7909,7909.11,7910,7910.11,7910.12,7911,7911.11,7911.12,791 2,7912.11,7912.12,7913,7913.11,7913.12,7914,7914.11,7915,7916,7916.11,7917,7917.11,79 18,7920,7920.11,7921,7921.11,7922,7922.11,7923,7923.11,7924,7925,7925.11,7926,7927,7 930,7931,7932,7933,7934,8735,7900000,7901000,7901100,7901200,7901400,7901500,7902 000,7902100,7902300,7902400,7902500,7903000,7903100,7904000,7905000,7905100,7906 000,7906100,7906111,7906200,7906300,7906400,7906500,7907000,7907011,7907100,7907 200,7907300,7907400,7908000,7908100,7908111,7908200,7908300,7908311,7908511,7909 000,7909100,7909300,7910000,7910100,7910200,7910211,7910212,7910213,7910214,7910 300,7910400,7910411,7911000,7911100,7911100,7911300,7911300,7911400,7911411,7912000,7912 100,7912200,7912300,7912511,7913000,7913100,7913200,7913300,7913400,7913411,7914 000,7914000,7914100,7914100,7914200,7914200,7914211,7914211,7914212,7914212,7914 300,7914300,7914400,7914500,7915000,7915100,7915200,7915300,7916000,7916100,7916 200,7916300,7917000,7917100,7917300,7917311,7918000,7918100,7918111,7918200,7918 300,7918400,7918500,7920000,7920100,7920200,7920300,7921000,7921100,7921200,7921 300,7922000,7922100,7922200,7922300,7923000,7923100,7923200,7923300,7924000,7924 100,7924200,7924500,7925000,7925011,7925012,7925100,7925200,7925400,7926000,7926 200,7926300,7927000,7927100,7927200,7927300,7927400,7927500,7930000,7930100,7930 200,7930300,7930400,7931000,7931100,7931200,7932000,7932100,7932111,7932200,7932 400,7932500,7933000,7933300,7934000,7934100,7934400,7934600,7934800,7.90E100,7.90 E111,7.90E200,7.90E211,14N6.00,14S4.00,14S4.00,14T3.00,14T3.00,79..00,79..11,790..0 0,7900z00,7901y00,7901z00,7902y00,7902z00,7903y00,7903z00,7904y00,7904z00,7905z0 0,7906y00,7906z00,7907y00,7907z00,7908y00,7908z00,7909y00,7909z00,790A.00,790A00 0,790A100,790A111,790A300,790A600,790Ay00,790Az00,790B.00,790B000,790B011,790 B012,790B100,790By00,790Bz00,790D.00,790D200,790D400,790D700,790E.00,790E500, 790Ey00,790Ez00,790F.00,790F000,790F100,790G.00,790G000,790G100,790Gy00,790H0 00,790H100,790H200,790H300,790H400,790H500,790Hy00,790Hz00,790J.00,790J000,790 K.00,790K200,790M.00,790M100,790M100,790M400,790M500,790Mz00,790N.00,790N000,790N2 0,790N300,790N400,790N500,790Ny00,791..00,7910y00,7910z00,7911y00,7911z00,7912y 00,7912z00,7913y00,7913z00,7914y00,7914z00,7915y00,7916y00,7916z00,7916z11,7917z 00,7918y00,7918z00,791A.00,791A000,791A100,791A200,791A300,791B.00,791B000,791 B100,791B200,791B400,791B500,791By00,791Bz00,791C.00,791C200,791C300,791C400, 791C500,791Cy00,791D.00,791D000,791D100,791y.00,791z.00,792..00,792..11,7920y00,7 920z00,7921y00,7921z00,7922y00,7922z00,7923z00,7924y00,7924z00,7925y00,7925z00,7 926z00,7927y00,7927z00,792B.00,792B000,792B100,792B200,792By00,792Bz00,792C.00,	36,45,61,94,188,7 63,786,792,805,83 3,1119,1291,1572, 1573,1781,2302,2 511,3058,3181,32 86,3691,3705,400 4,5441,5858,6262, 6751,7445,7465,8 060,8061,8466,84 67,8749,8832,918 8,9292,9522,1068 7,10871,11380,12 322,12456,13051, 13348,13434,1348 7,13549,14856,15 042,15313,16366, 17119,17679,1796 5,20844,20944,23 078,24635,25238, 27161,27193,2752 3,27727,29024,29 282,29456,30047, 30202,30203,3099 0,31079,31209,31 511,31937,32109, 32164,32553,3308 0,33119,33274,33 391,33578,33612, 33675,33711,3401 7,34019,34023,34 024,34086,34087, 34088,34095,3429 9,34327,34328,34 371,34416,34417, 34418,34515,3451

				K464,K465,K468,K469,K47,K471,K472,K473,K474,K475,K478,K479,K48,K481,K482,K483,K484,K488,K489,K52,K521,K522,K523,K524,K525,K526,K528,K529,K53,K531,K532,K538,K539,K54,K541,K542,K548,K549,K55,K551,K552,K553,K554,K555,K556,K558,K559,K56,K561,K562,K563,K564,K568,K569,K57,K571,K572,K573,K574,K575,K576,K577,K578,K579,K62,K66,K661,K668,K669,K67,K671,K678,K679,X501,X502,X504	792C000,792Cy00,792Cz00,792D.00,792Dy00,792Dz00,792y.00,792z.00,7930y00,7930z00,7932z00,7933z00,7934y00,7934z00,793A.00,793A.11,793A000,793A100,793Az00,793E.00,793Ey00,793Ez00,793H.00,793Hy00,793L.00,793L000,793L100,793M100,79y..00,79z..00,7L1H200,7M36000,7N4..00,7N40.00,7N40000,7N40100,7N40200,7N40300,7N41400,7N41500,7N41600,8H2O.00,9b8B.00,G573.00,G573000,G573100,G573200,G573300,G573400,G573500,G573z00,P512.00,SP00200,SyuK611,TB01200,ZV15100,ZV42100,ZV42200,ZV42200,ZV43300,ZV43300,ZV45800,ZV45H00,ZV45H00,ZV45K00,ZV45K11,ZV59600,ZVu6e00	7,34519,34520,34526,34574,34576,34600,34640,34690,34691,34751,34758,34759,34851,34864,34918,34948,35517,35520,35710,36099,38041,38044,38498,39423,39866,40055,40143,40245,41530,41551,41735
Type 2 diabetes			E10, E11, E12, O242, E13, E14, G590, G632, H280, H360, M142, N083, O240, O241, O243	66An.00,C100000,C100011,C101000,C102000,C103000,C104000,C105000,C106000,C107000,C107300,C108.00,C108.11,C108.12,C108.13,C108000,C108011,C108012,C108100,C108200,C108211,C108212,C108300,C108400,C108411,C108412,C108500,C108511,C108512,C108600,C108700,C108711,C108712,C108800,C108811,C108812,C108900,C108911,C108912,C108A00,C108A11,C108B00,C108C00,C108D00,C108D11,C108E00,C108E11,C108E12,C108F00,C108F11,C108G00,C108H00,C108H11,C108J00,C108J11,C108J12,C10C.12,C10E.00,C10E.11,C10E.12,C10E000,C10E100,C10E112,C10E200,C10E300,C10E311,C10E312,C10E400,C10E411,C10E412,C10E500,C10E511,C10E512,C10E600,C10E700,C10E711,C10E712,C10E800,C10E812,C10E900,C10E911,C10E912,C10EA00,C10EA11,C10EB00,C10EC00,C10EC11,C10ED00,C10EE00,C10EF00,C10EG00,C10EH00,C10EJ00,C10EK00,C10EL00,C10EM00,C10EM11,C10EN00,C10EN11,C10EP00,C10EP11,C10EQ00,C10z000,L180500,M21yC00,M21yC11,ZC2C900,ZRbH.00,66A0.00,C100100,C100111,C100112,C101100,C102100,C103100,C104100,C105100,C106100,C107100,C107200,C107400,C109.00,C109.11,C109.12,C109.13,C109000,C109011,C109012,C109100,C109111,C109112,C109200,C109211,C109212,C109300,C109400,C109411,C109412,C109500,C109511,C109512,C109600,C109611,C109612,C109700,C109711,C109712,C109900,C109A00,C109A11,C109B00,C109B11,C109C00,C109C11,C109C12,C109D00,C109D11,C109D12,C109E00,C109E11,C109E12,C109F00,C109F11,C109F12,C109G00,C109G11,C109G12,C109H00,C109H11,C109H12,C109J00,C109J11,C109J12,C109K00,C10C.11,C10D.00,C10D.11,C10ER00,C10F.00,C10F.11,C10F000,C10F011,C10F100,C10F200,C10F211,C10F300,C10F311,C10F400,C10F411,C10F500,C10F600,C10F611,C10F700,C10F711,C10F900,C10F911,C10FA00,C10FA11,C10FB00,C10FB11,C10FC00,C10FD00,C10FD11,C10FE00,C10FE11,C10FF00,C10FG00,C10FH00,C10FJ00,C10FJ11,C10FK00,C10FL00,C10FL11,C10FM00,C10FM11,C10FN00,C10FP00,C10FQ00,C10FR00,C10y100,C10z100,L180600,ZC2CA00		
Hypertension	Documented systolic blood pressure >140mmHg or diastolic blood pressure >90mmHg before baseline					

Table S2. GWAS summary statistics data source

Trait	Description	Cohort / Consortium	Imputation reference	Study-level association testing	Study	URL
Body mass index	a multi-ancestry GWAS meta-analysis of body mass index from 694,649 participants of European ancestry.	GIANT + UK Biobank	HapMap2, HRC	Linear mixed model with rank-based inverse-normal transformed phenotype	Pulit S et al (2019)	https://doi.org/10.1093/hmg/ddy327
Heart failure	a GWAS meta-analysis of 47,309 heart failure cases and 930,014 controls from 26 cohorts of European ancestry	HERMES	1000G (Phase 1 and 3), HapMap2, HRC, population-specific reference	Logistic regression + cox proportional hazard (for incident cases)	Shah et al (2020)	https://doi.org/10.1038/s41467-019-13690-5
Coronary artery disease	a multi-ancestry GWAS meta-analysis of 60,801 CAD cases and 123,504 controls from 48 studies	CARDIoGRAMplusC4D	1000G Phase1 v3	Logistic regression	Nikpay et al (2015)	https://doi.org/10.1038/ng.3396
Atrial fibrillation	a multi-ancestry GWAS meta-analysis of 65,446 AF cases and more than 522,000 controls from more than 50 studies	AFGen	HRC v1.1, 1000G Phase1 v3, population-specific reference	Logistic regression + cox proportional hazard (for incident cases)	Roselli et al (2018)	https://doi.org/10.1038/s41588-018-0133-9
Type 2 diabetes	a GWAS meta-analysis of 74,124 type 2 diabetes cases and 824,006 controls of European ancestry.	DIAGRAM	HRC, population-specific reference	Logistic regression + linear mixed model	Mahajan A et al (2018)	https://doi.org/10.1038/s41588-018-0241-6
Systolic and diastolic blood pressure	a GWAS conducted in 329,985 UK Biobank participants of European ancestry. Participants with extreme systolic blood pressure measurement (outside ± 7 SD) and had used blood pressure lowering drugs according to self-reported medication data were excluded.	UK Biobank	HRC	Linear mixed model adjusted for 10 genetic principal components using standardised phenotypes and pre-adjusted for sex and age	in-house data	

Table S3. Multivariable Mendelian randomization (MVMR) analysis results for association of body mass index (BMI) with heart failure (HF)

A. Correlated instruments were selected for instrument with lowest P-value for association with BMI

Method	Covariates	N instrument	beta	SE	OR	OR Lower 95% CI	OR Upper 95% CI
IVW	-	1684	0.4958	0.0180	1.6418	1.5848	1.7009
MR-Egger	-	1684	0.4740	0.0502	1.6065	1.4559	1.7725
WME	-	1684	0.5220	0.0278	1.6855	1.5961	1.7799
MVMR-IVW	AF	1210	0.4503	0.0218	1.5687	1.5030	1.6373
MVMR-Egger	AF	1210	0.4923	0.0519	1.6361	1.4778	1.8113
MVMR-IVW	CAD	1154	0.4166	0.0225	1.5167	1.4514	1.5850
MVMR-Egger	CAD	1154	0.3683	0.0564	1.4453	1.2939	1.6143
MVMR-IVW	T2D	1201	0.4273	0.0275	1.5331	1.4526	1.6181
MVMR-Egger	T2D	1201	0.3680	0.0640	1.4448	1.2744	1.6379
MVMR-IVW	SBP	1313	0.4610	0.0231	1.5856	1.5156	1.6589
MVMR-Egger	SBP	1313	0.5002	0.0484	1.6490	1.4997	1.8132
MVMR-IVW	AF,CAD,T2D,SBP	1492	0.3219	0.0262	1.3798	1.3107	1.4525
MVMR-Egger	AF,CAD,T2D,SBP	1492	0.2951	0.0488	1.3433	1.2207	1.4782

B. Correlated instruments were selected at random

Method	Covariates	N instrument	beta	SE	OR	OR Lower 95% CI	OR Upper 95% CI
IVW	-	1684	0.4958	0.0180	1.6418	1.5848	1.7009
MR-Egger	-	1684	0.4740	0.0502	1.6065	1.4559	1.7725
WME	-	1684	0.5220	0.0278	1.6855	1.5961	1.7799
MVMR-IVW	AF	1209	0.4490	0.0219	1.5668	1.5008	1.6356
MVMR-Egger	AF	1209	0.4790	0.0514	1.6145	1.4597	1.7857
MVMR-IVW	CAD	1153	0.4082	0.0225	1.5040	1.4391	1.5719
MVMR-Egger	CAD	1153	0.3715	0.0569	1.4499	1.2968	1.6211
MVMR-IVW	T2D	1195	0.4289	0.0277	1.5356	1.4546	1.6211
MVMR-Egger	T2D	1195	0.3652	0.0632	1.4409	1.2730	1.6309
MVMR-IVW	SBP	1309	0.4597	0.0236	1.5837	1.5122	1.6586
MVMR-Egger	SBP	1309	0.5126	0.0490	1.6697	1.5168	1.8380
MVMR-IVW	AF,CAD,T2D,SBP	1481	0.3301	0.0271	1.3911	1.3191	1.4670
MVMR-Egger	AF,CAD,T2D,SBP	1481	0.2962	0.0516	1.3447	1.2154	1.4877

Estimates shown in the table represent effect of BMI on HF independent of covariates shown in the Covariates column. Covariates "-" represent results from univariate MR analysis. Beta: effect estimate (log odds) for BMI; SE: standard error of the effect estimate; OR: odds ratio; CI: confidence interval; IVW: inverse-variance weighted, MR-Egger: Mendelian Randomisation-Egger, WME: weighted median estimator, MVMR: multivariable Mendelian Randomisation; AF: atrial fibrillation; CAD: coronary artery disease; T2D: type 2 diabetes; SBP: systolic blood pressure.

Table S4. Mendelian Randomization Pleiotropy RESidual Sum and Outlier (MR-PRESSO) analysis results for association of body mass index (BMI) with heart failure (HF)

Method	Covariates	N outlier	beta	SE	OR	OR Lower 95% CI	OR Upper 95% CI	P-value
MR-PRESSO Raw	-	4	0.5031	0.0220	1.6539	1.5841	1.7268	4.68E-95
MR-PRESSO Outlier-corrected	-	4	0.5115	0.0216	1.6678	1.5988	1.7398	7.53E-101
MR-PRESSO Raw	AF	1	0.4505	0.0218	1.5691	1.5034	1.6377	3.26E-81
MR-PRESSO Outlier-corrected	AF	1	0.5038	0.0236	1.6550	1.5801	1.7336	1.14E-85
MR-PRESSO Raw	CAD	0	0.4166	0.0225	1.5167	1.4514	1.5850	3.48E-67
MR-PRESSO Outlier-corrected	CAD	0						
MR-PRESSO Raw	T2D	1	0.4283	0.0275	1.5347	1.4542	1.6197	4.60E-49
MR-PRESSO Outlier-corrected	T2D	1	0.5100	0.0247	1.6653	1.5865	1.7481	9.22E-79
MR-PRESSO Raw	SBP	1	0.4606	0.0230	1.5850	1.5151	1.6580	8.96E-78
MR-PRESSO Outlier-corrected	SBP	1	0.5060	0.0230	1.6586	1.5856	1.7350	2.50E-91
MR-PRESSO Raw	AF,CAD,T2D,SBP	0	0.3237	0.0262	1.3822	1.3131	1.4549	3.77E-33
MR-PRESSO Outlier-corrected	AF,CAD,T2D,SBP	0						

Table S5. Univariate Mendelian randomization (MR) analysis results for association of BMI with heart failure outcome adjusted using mtCoJo at summary statistics.

Method	mtCOJO adjustment	beta	SE	OR	OR Lower 95% CI	OR Upper 95% CI	P-value
IVW	Unadjusted	0.4958	0.0180	1.6418	1.5848	1.7009	2.67E-166
MR-Egger	Unadjusted	0.4740	0.0502	1.6065	1.4559	1.7725	3.61E-21
WME	Unadjusted	0.5220	0.0278	1.6855	1.5961	1.7799	1.24E-78
IVW	AF	0.4523	0.0175	1.5720	1.5189	1.6269	6.83E-147
MR-Egger	AF	0.4244	0.0488	1.5286	1.3893	1.6819	3.28E-18
WME	AF	0.4672	0.0273	1.5955	1.5123	1.6833	1.76E-65
IVW	CAD	0.3826	0.0181	1.4661	1.4149	1.5191	6.74E-99
MR-Egger	CAD	0.3123	0.0504	1.3666	1.2380	1.5086	5.92E-10
WME	CAD	0.3808	0.0285	1.4634	1.3840	1.5475	9.22E-41
IVW	T2D	0.4455	0.0205	1.5613	1.4999	1.6251	3.58E-105
MR-Egger	T2D	0.4398	0.0615	1.5524	1.3762	1.7512	8.44E-13
WME	T2D	0.4638	0.0329	1.5901	1.4908	1.6960	3.76E-45
IVW	SBP	0.5086	0.0181	1.6629	1.6051	1.7228	1.60E-174
MR-Egger	SBP	0.4981	0.0520	1.6455	1.4861	1.8221	9.99E-22
WME	SBP	0.5247	0.0283	1.6900	1.5989	1.7863	7.01E-77
IVW	AF,CAD,T2D,SBP	0.4470	0.0204	1.5636	1.5024	1.6273	1.02E-106
MR-Egger	AF,CAD,T2D,SBP	0.3937	0.0612	1.4825	1.3150	1.6713	1.21E-10
WME	AF,CAD,T2D,SBP	0.4288	0.0322	1.5354	1.4413	1.6355	2.39E-40

Beta: effect estimate (log odds) for BMI;

SE: standard error of the effect estimate;

OR: odds ratio;

CI: confidence interval;

IVW: inverse-variance weighed,

MR-Egger: Mendelian Randomisation-Egger

WME: weighted median estimator,

AF: atrial fibrillation;

CAD: coronary artery disease;

T2D: type 2 diabetes;

SBP: systolic blood pressure

SUPPLEMENTARY FIGURES

Figure S1. Flow chart for specification of the study population

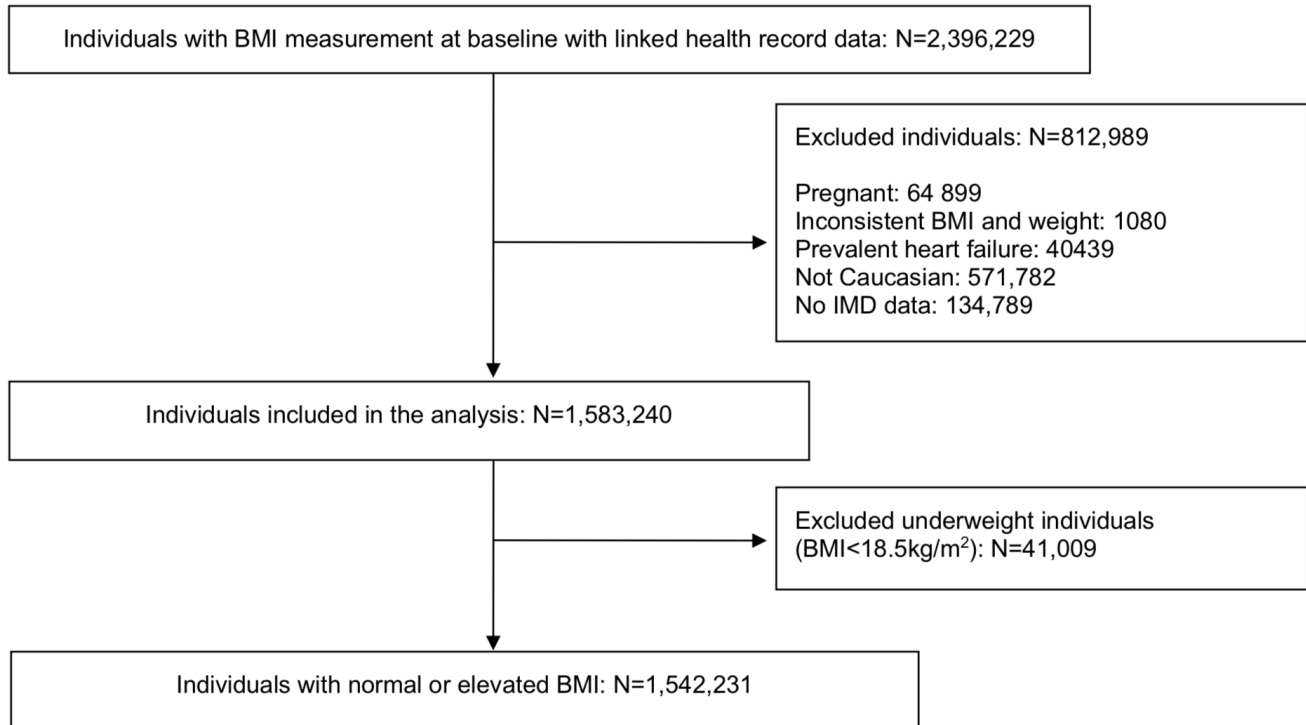


Figure S2. Observational association of body mass index categories with incident heart failure in 1,583,240 individuals. Estimated hazard ratios for body mass index (BMI) on incident heart failure, adjusted for age and sex. Hazard ratios are given per 4.807 kg/m² increase in BMI, equating to the standard deviation of BMI in UK Biobank.

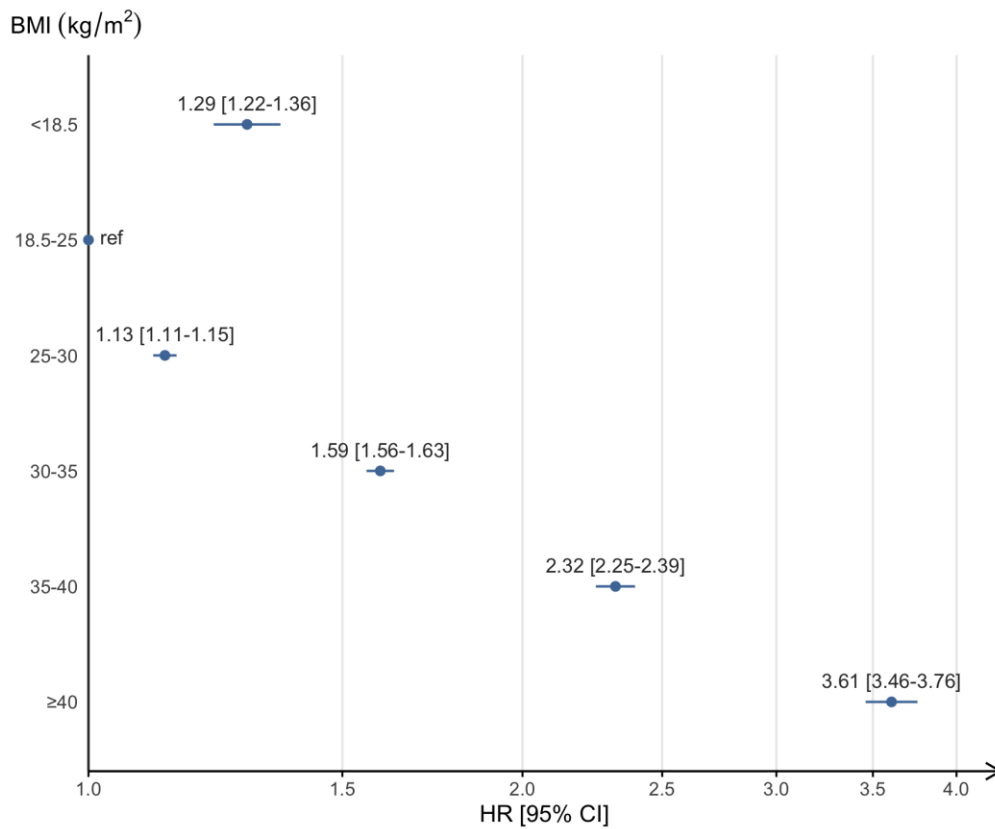


Figure S3. Sensitivity analyses for phenotypic association of body mass index with incident heart failure. **A.** Sex stratified analyses adjusted for age and sex (base model), and additional risk factors. **B.** All sample analyses adjusted for age, sex, Index of Multiple Deprivation (base model), and additional risk factors. **C.** Analyses excluding participants with incident heart failure in the first 2 year, adjusted for age and sex (base model), and additional risk factors. For all panels, points and error bars represent adjusted hazard ratios and 95% confidence interval for the effects of body mass index (BMI) on incident heart failure. Hazard ratios are given per 4.807 kg/m² increase in BMI, corresponding to the approximate standard deviation of the sample used for genetic inference analyses. HTN, hypertension; AF, atrial fibrillation; CHD, coronary heart disease; DM, diabetes mellitus.

